

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100623\
Data File : FG013013.D
Signal(s) : FID1A.ch
Acq On : 06 Oct 2023 13:58
Operator : YP\AJ
Sample : PB156174BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 07 01:49:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092123.M
Quant Title :
QLast Update : Fri Sep 22 02:14:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.075	1960482	17.299 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.275	73836	0.616 ug/ml
13) N-TRIACONTANE	18.141	53574	0.464 ug/ml
14) N-DOTRIACONTANE	18.974	59220	0.532 ug/ml
15) N-TETRATRIACONTANE	19.758	53923	0.571 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100623\
Data File : FG013013.D
Signal(s) : FID1A.ch
Acq On : 06 Oct 2023 13:58
Operator : YP\AJ
Sample : PB156174BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 07 01:49:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092123.M
Quant Title :
QLast Update : Fri Sep 22 02:14:31 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

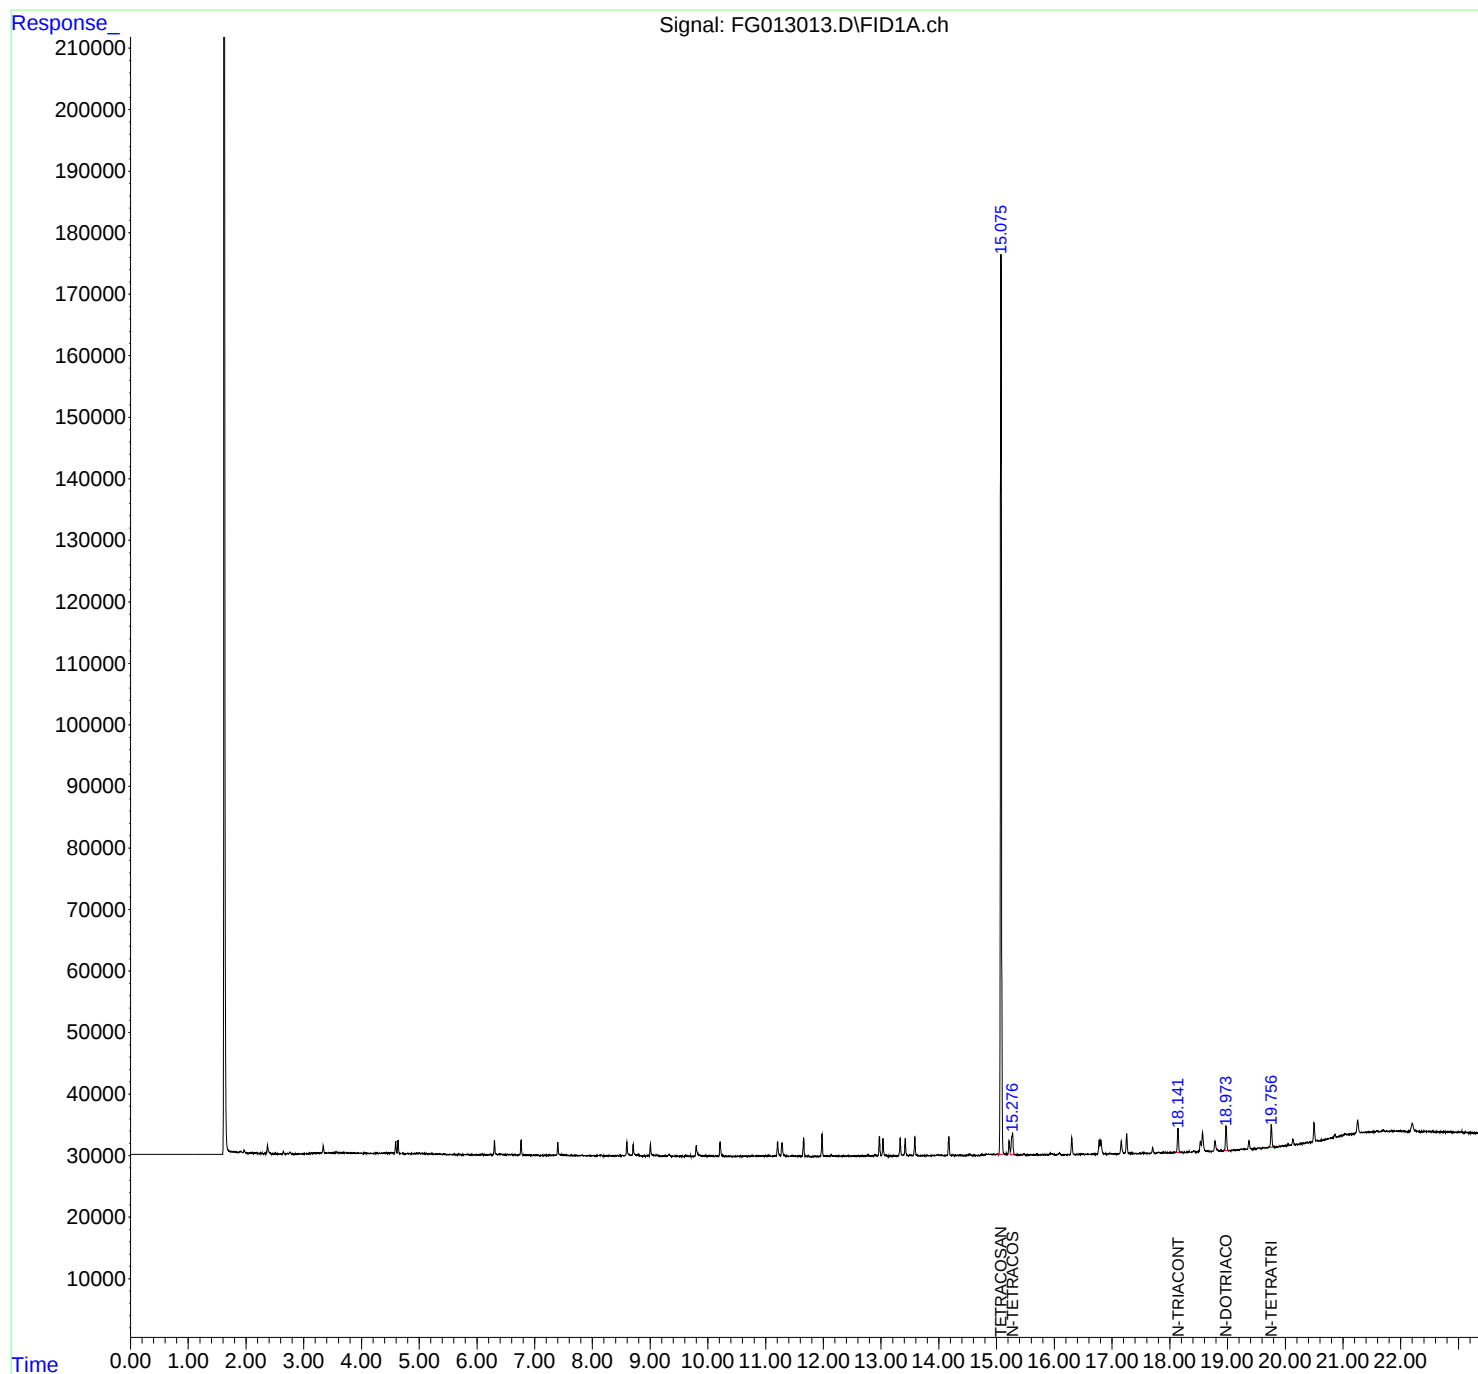

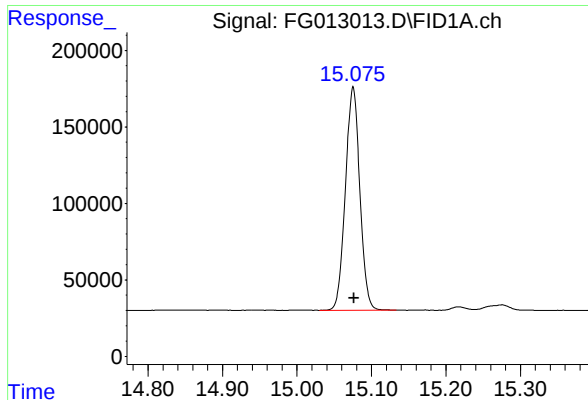


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.075 min
Delta R.T.: -0.001 min
Response: 1960482
Conc: 17.30 ug/ml

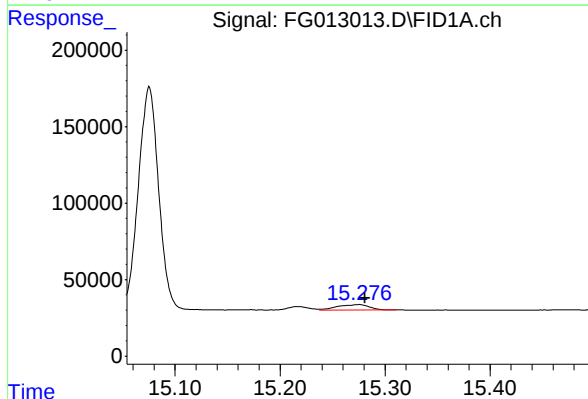


#10 N-TETRACOSANE

R.T.: 15.275 min
Delta R.T.: -0.005 min
Response: 73836
Conc: 0.62 ug/ml

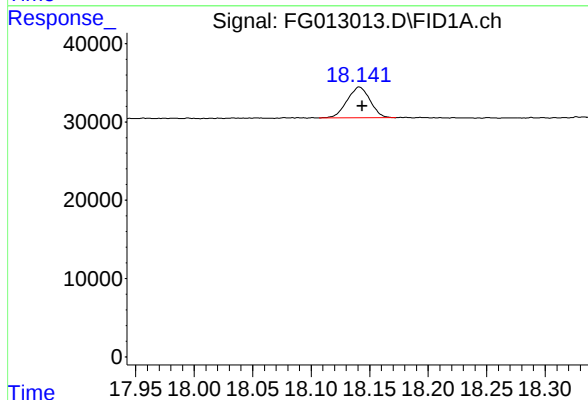


#13 N-TRIACONTANE

R.T.: 18.141 min
Delta R.T.: -0.002 min
Response: 53574
Conc: 0.46 ug/ml

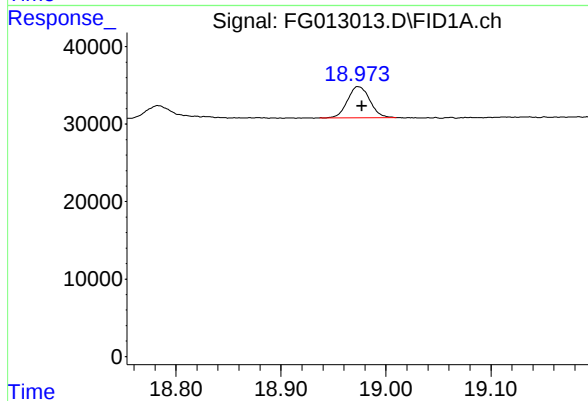

#14 N-DOTRIACONTANE

R.T.: 18.974 min
Delta R.T.: -0.003 min
Response: 59220
Conc: 0.53 ug/ml

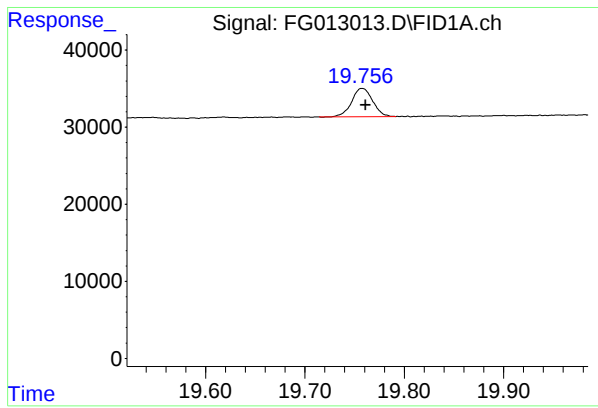

#15 N-TETRATRIACONTANE

R.T.: 19.758 min
Delta R.T.: -0.003 min
Response: 53923
Conc: 0.57 ug/ml