

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100721\
Data File : FG008799.D
Signal(s) : FID1A.ch
Acq On : 07 Oct 2021 14:50
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 03:32:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.810	61569	0.543 ug/ml
14) N-DOTRIACONTANE	18.644	82529	0.778 ug/ml
15) N-TETRATRIACONTANE	19.426	62753	0.630 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100721\
Data File : FG008799.D
Signal(s) : FID1A.ch
Acq On : 07 Oct 2021 14:50
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 03:32:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

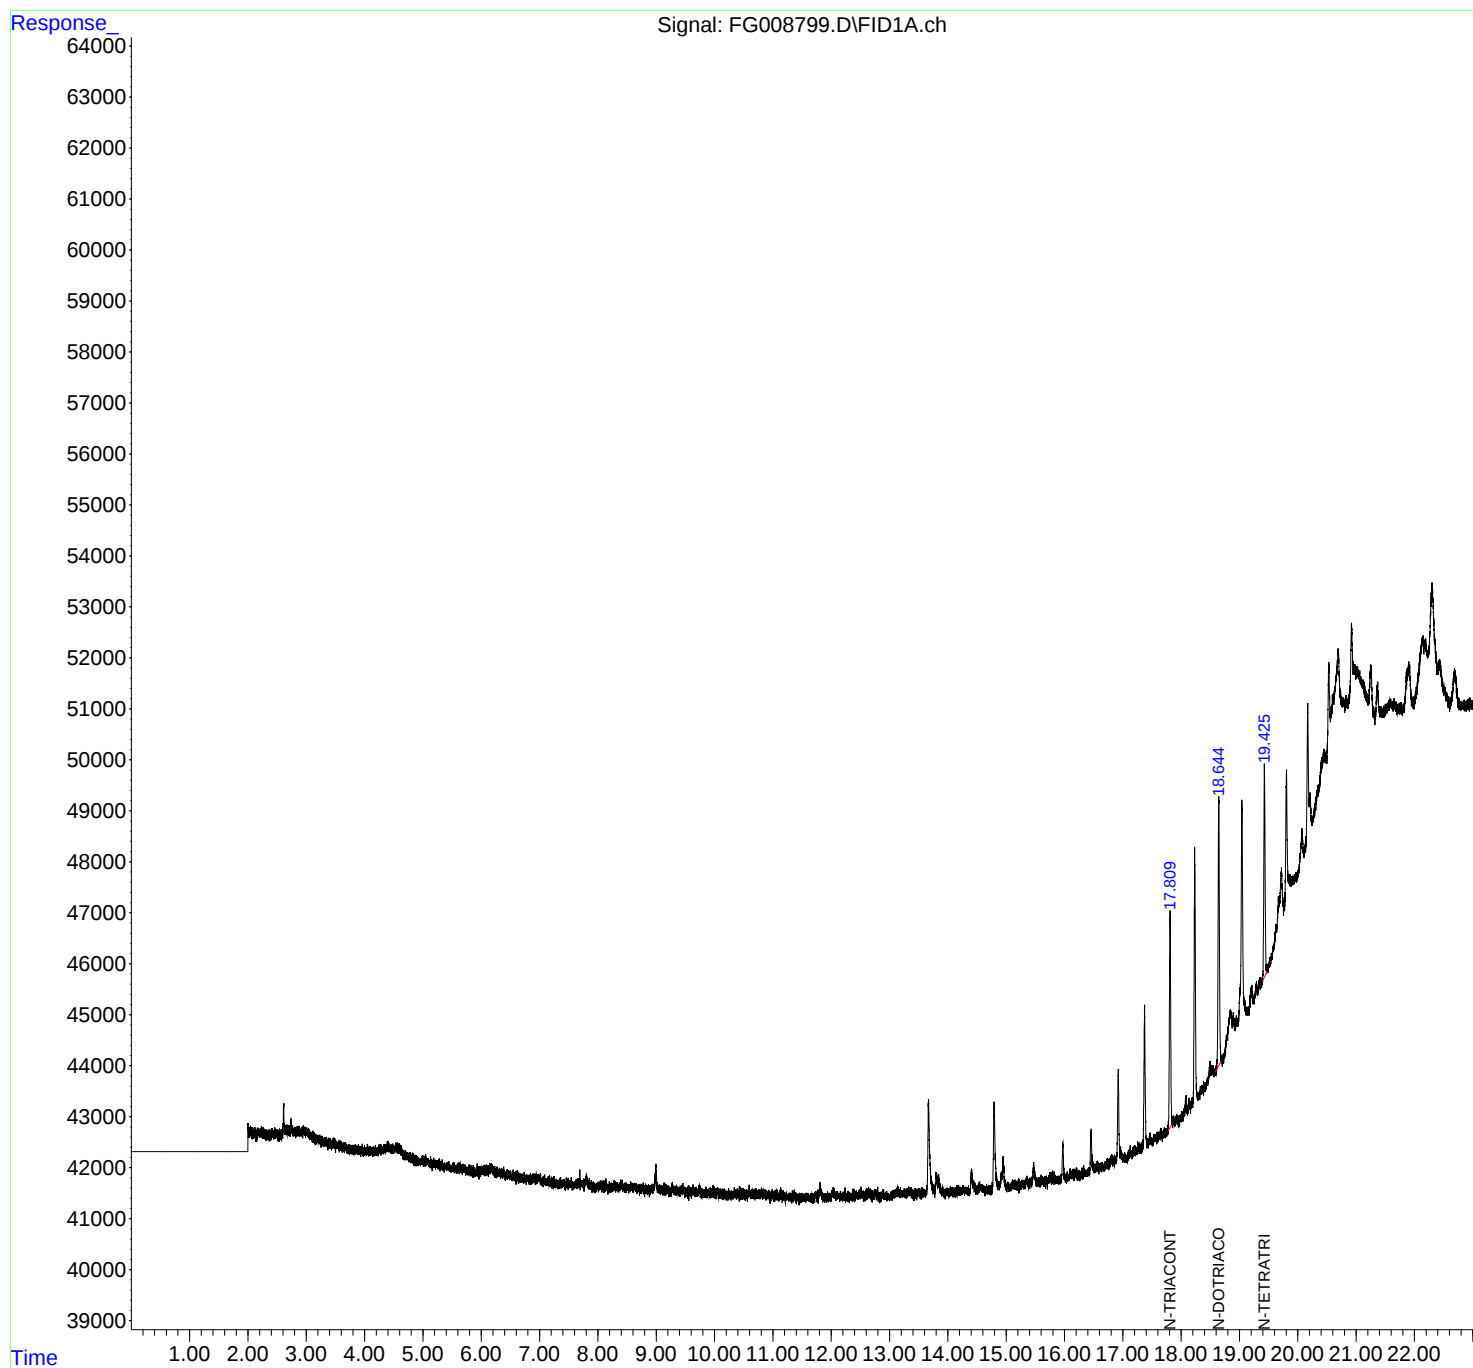


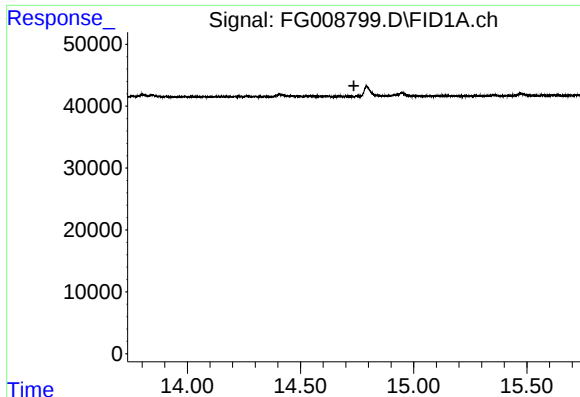

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.736 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

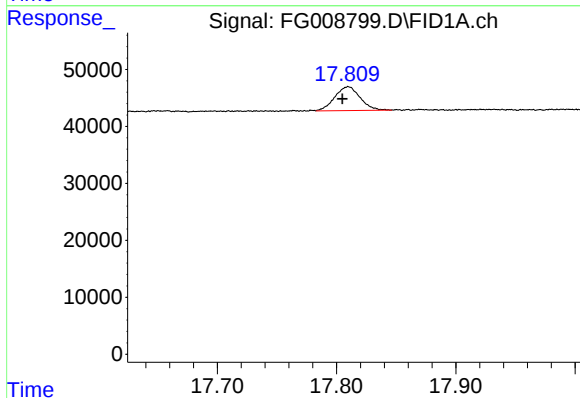


#13 N-TRIACONTANE

R.T.: 17.810 min
Delta R.T.: 0.005 min
Response: 61569
Conc: 0.54 ug/ml

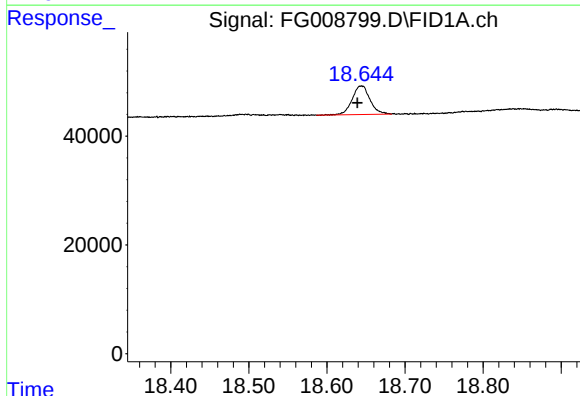

#14 N-DOTRIACONTANE

R.T.: 18.644 min
Delta R.T.: 0.005 min
Response: 82529
Conc: 0.78 ug/ml

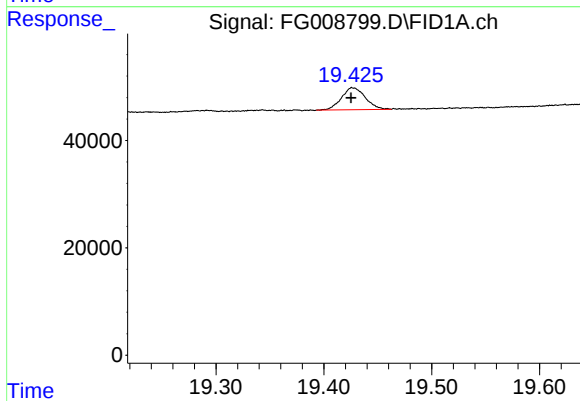

#15 N-TETRATRIACONTANE

R.T.: 19.426 min
Delta R.T.: 0.000 min
Response: 62753
Conc: 0.63 ug/ml