

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100722\
Data File : FG010826.D
Signal(s) : FID1A.ch
Acq On : 08 Oct 2022 00:26
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 20:27:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.738	2253530	18.575 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.636	301706	2.374 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100722\
Data File : FG010826.D
Signal(s) : FID1A.ch
Acq On : 08 Oct 2022 00:26
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 20:27:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

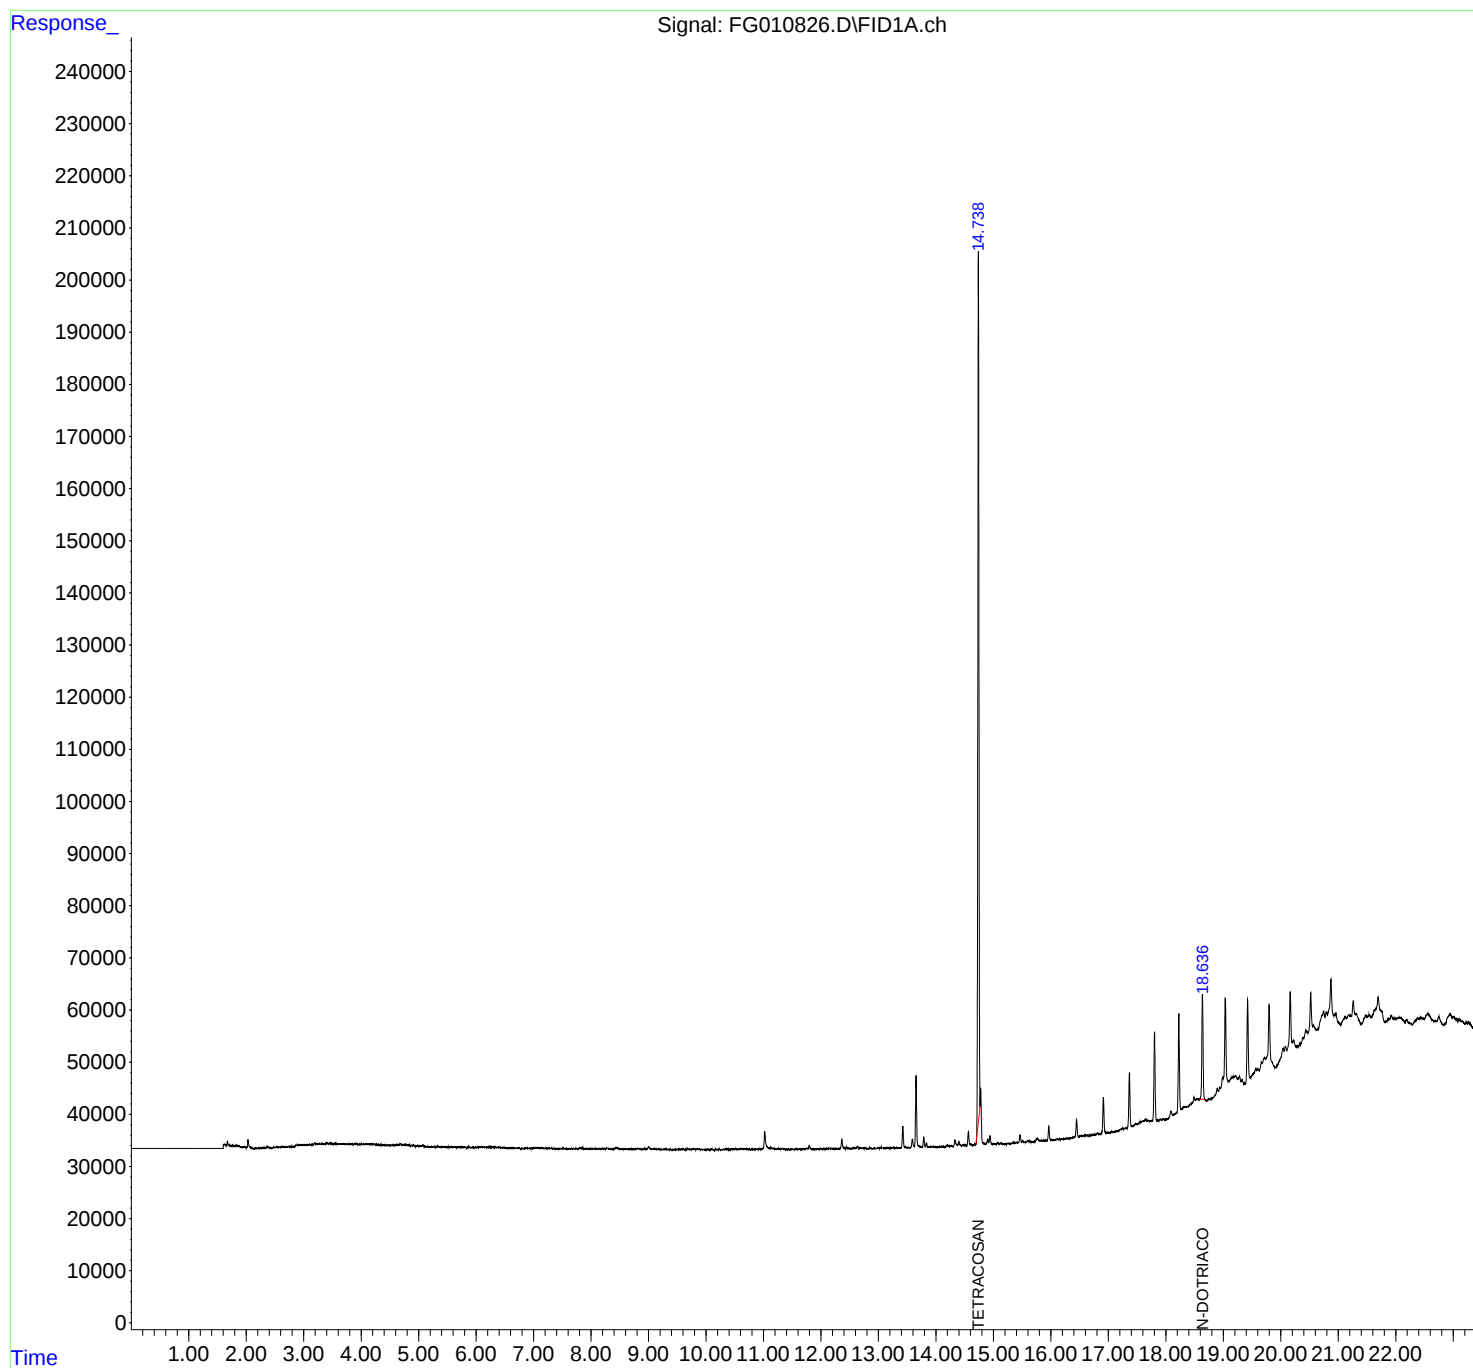


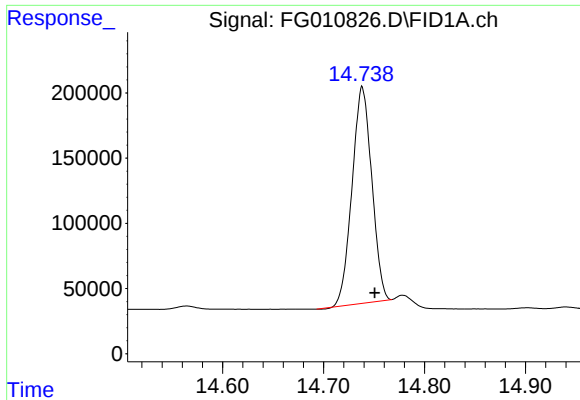

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: -0.012 min
Response: 2253530
Conc: 18.58 ug/ml

Instrument :
FID_G
ClientSampleId :

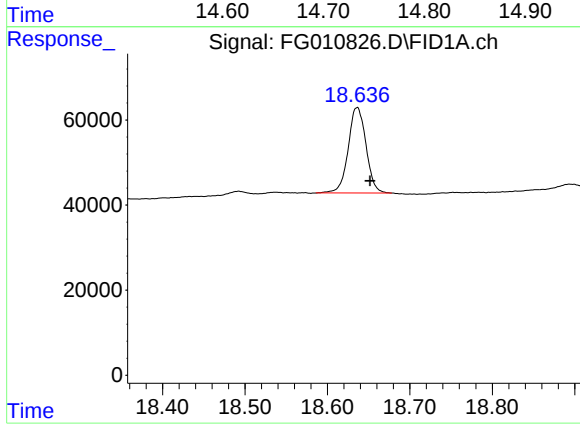

#14 N-DOTRIACONTANE

R.T.: 18.636 min
Delta R.T.: -0.016 min
Response: 301706
Conc: 2.37 ug/ml