

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG100722\  
Data File : FG010813.D  
Signal(s) : FID1A.ch  
Acq On : 07 Oct 2022 11:55  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Oct 08 19:48:49 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG092822.M  
Quant Title :  
QLast Update : Thu Sep 29 02:21:49 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.444  | 1705766  | 12.862 ug/ml |
| 12)                         | N-OCTACOSANE | 16.918 | 1806104  | 13.773 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG100722\  
Data File : FG010813.D  
Signal(s) : FID1A.ch  
Acq On : 07 Oct 2022 11:55  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Oct 08 19:48:49 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG092822.M  
Quant Title :  
QLast Update : Thu Sep 29 02:21:49 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

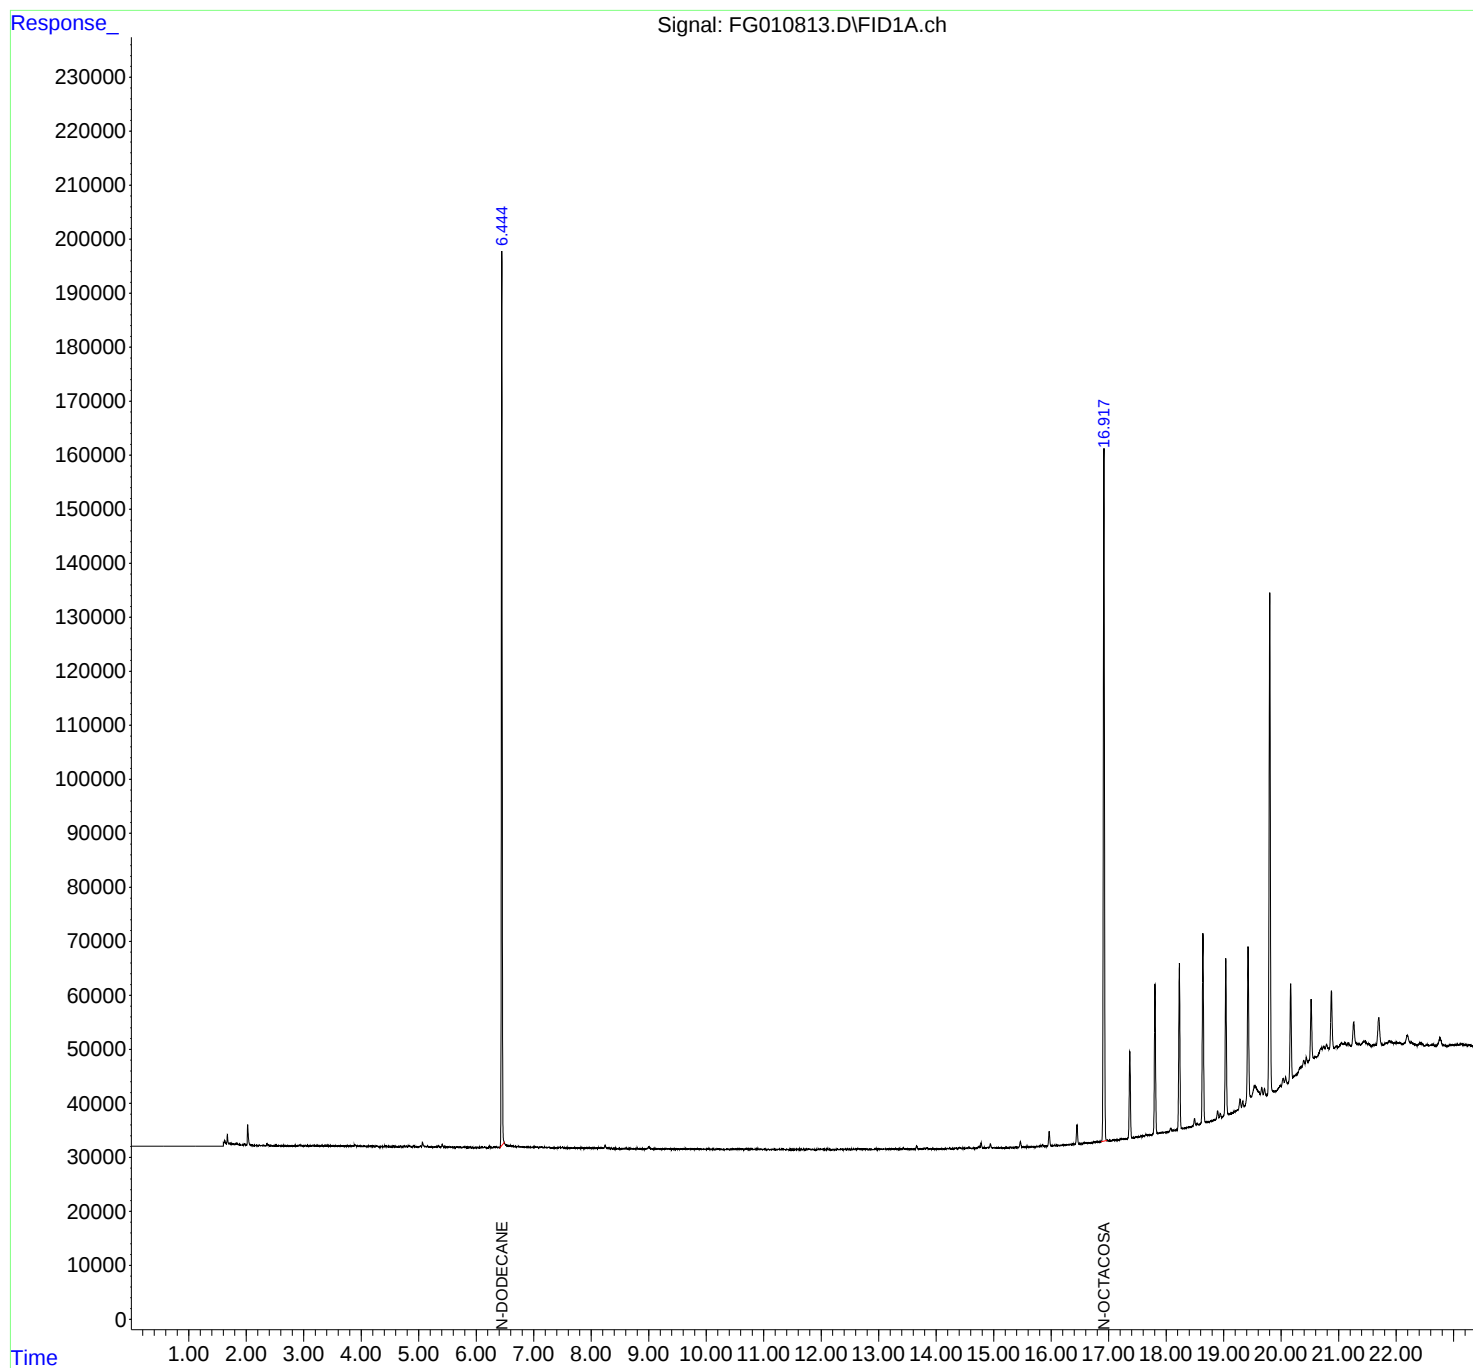


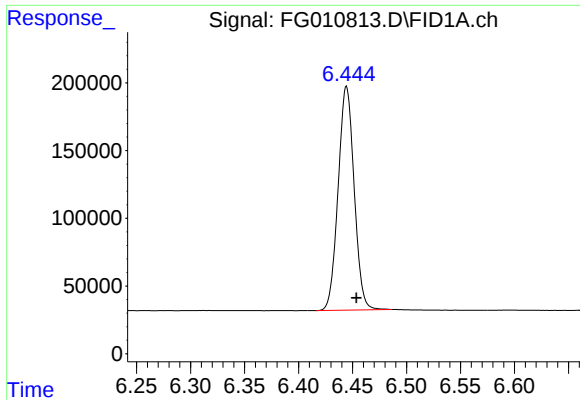

#3 N-DODECANE


R.T.: 6.444 min  
Delta R.T.: -0.009 min  
Response: 1705766  
Conc: 12.86 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
RT MARKER

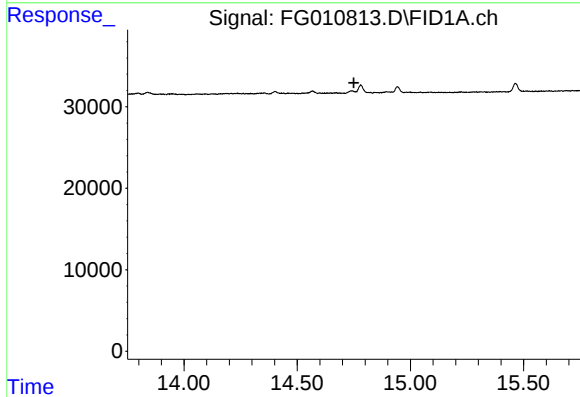

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.751 min  
Response: 0  
Conc: N.D.

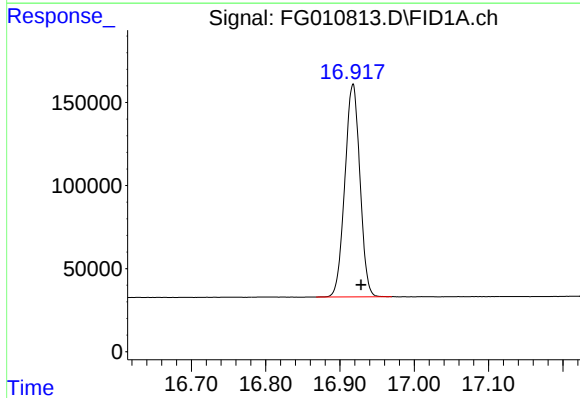

#12 N-OCTACOSANE

R.T.: 16.918 min  
Delta R.T.: -0.011 min  
Response: 1806104  
Conc: 13.77 ug/ml