

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100722\
Data File : FG010818.D
Signal(s) : FID1A.ch
Acq On : 07 Oct 2022 17:25
Operator : YP\AJ
Sample : N5018-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-T-3-(0-5)

Integration File: autoint1.e
Quant Time: Oct 08 19:49:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.741	1876685	15.469 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100722\
Data File : FG010818.D
Signal(s) : FID1A.ch
Acq On : 07 Oct 2022 17:25
Operator : YP\AJ
Sample : N5018-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-T-3-(0-5)

Integration File: autoint1.e
Quant Time: Oct 08 19:49:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

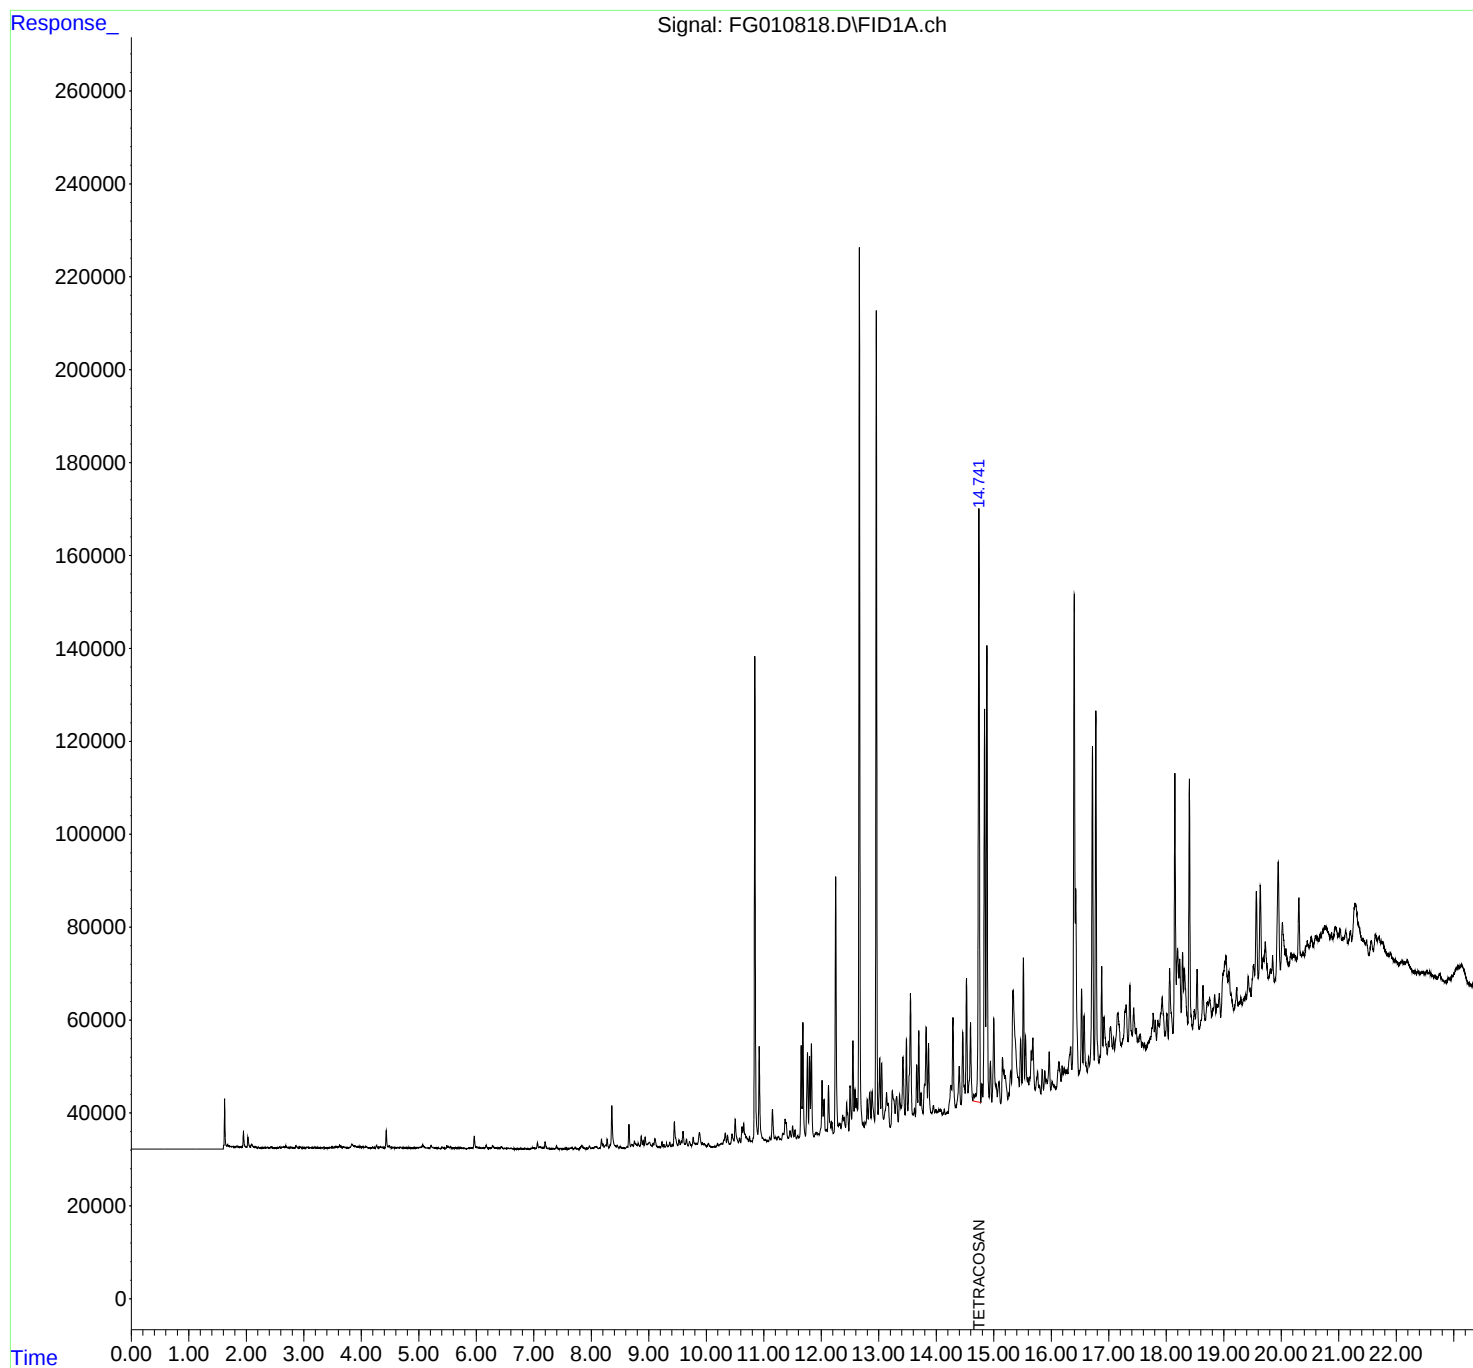

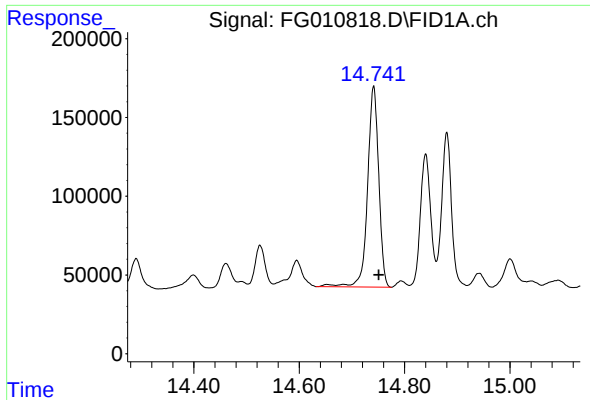

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.741 min
Delta R.T.: -0.009 min
Response: 1876685
Conc: 15.47 ug/ml

Instrument :
FID_G
ClientSampleId :
SASP2-T-3-(0-5)