

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100722\
Data File : FG010822.D
Signal(s) : FID1A.ch
Acq On : 07 Oct 2022 21:27
Operator : YP\AJ
Sample : N5018-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-T-3-(10-14)

Integration File: autoint1.e
Quant Time: Oct 08 19:49:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.739	2175005	17.928 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100722\
Data File : FG010822.D
Signal(s) : FID1A.ch
Acq On : 07 Oct 2022 21:27
Operator : YP\AJ
Sample : N5018-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-T-3-(10-14)

Integration File: autoint1.e
Quant Time: Oct 08 19:49:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

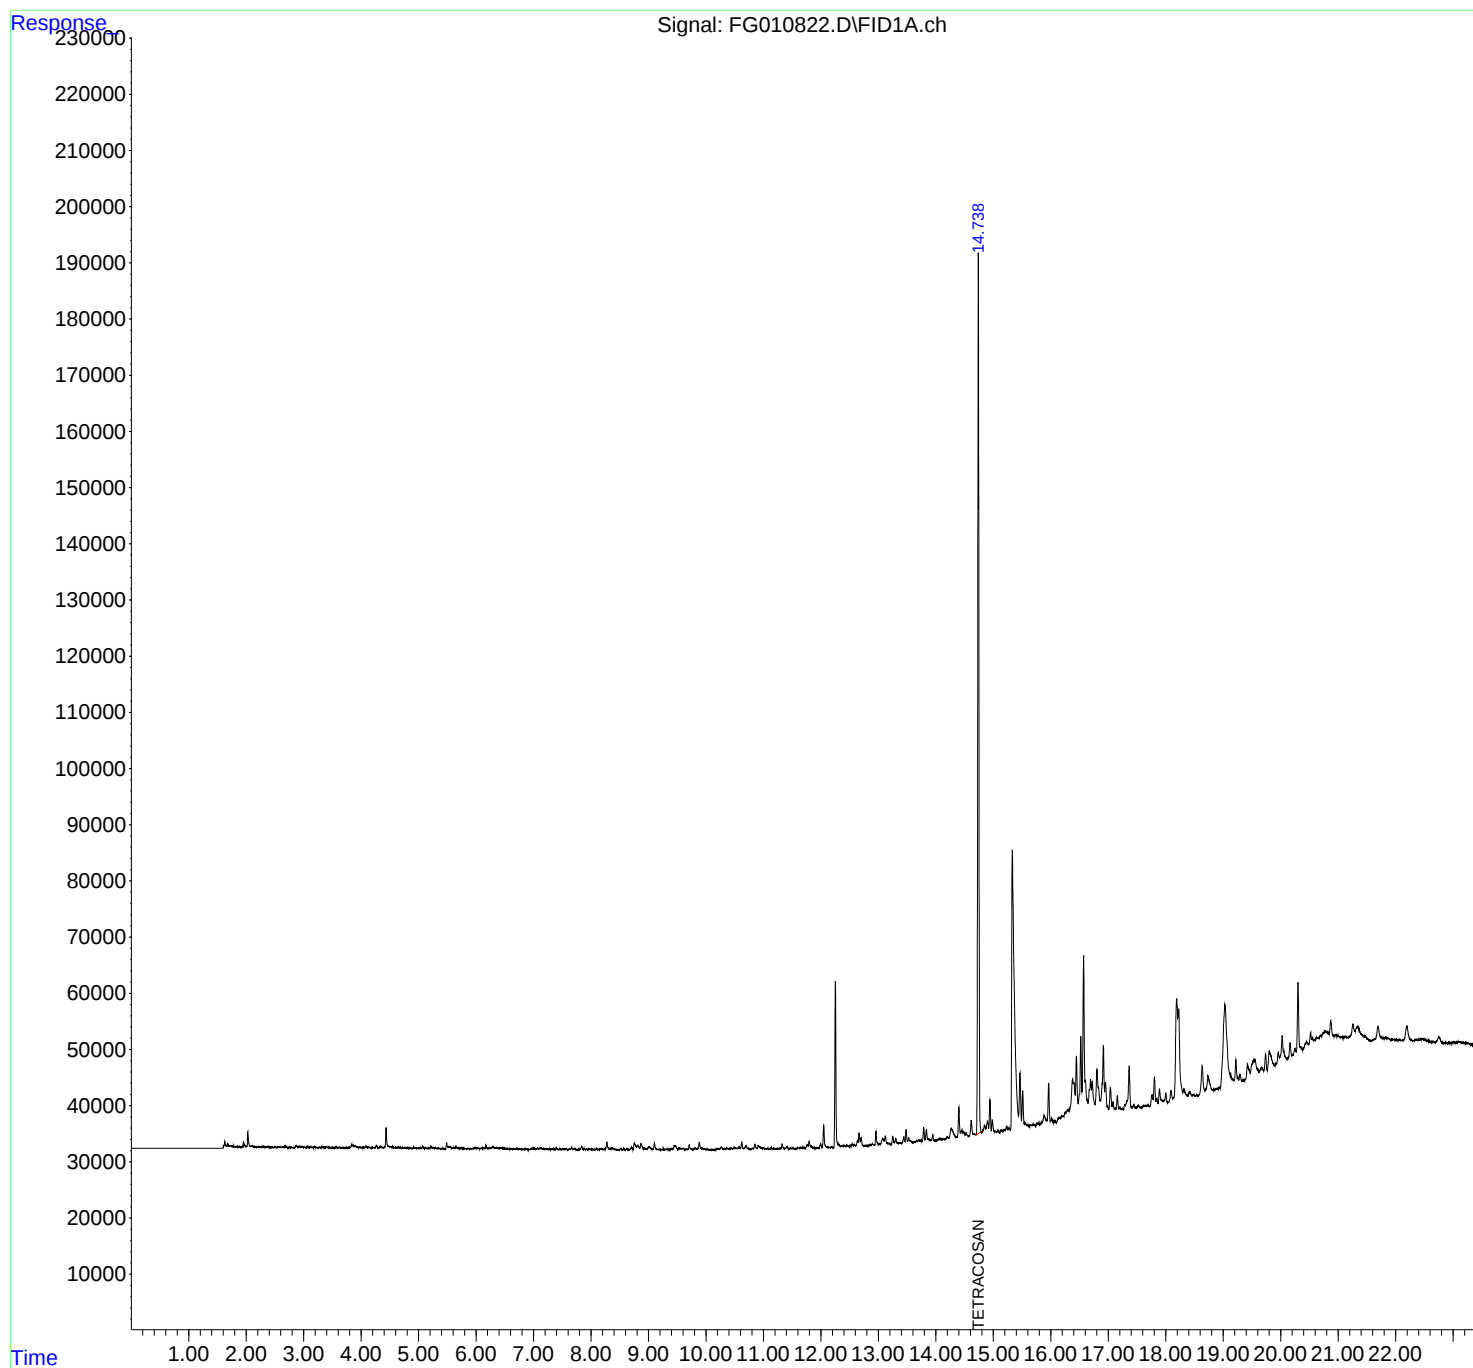

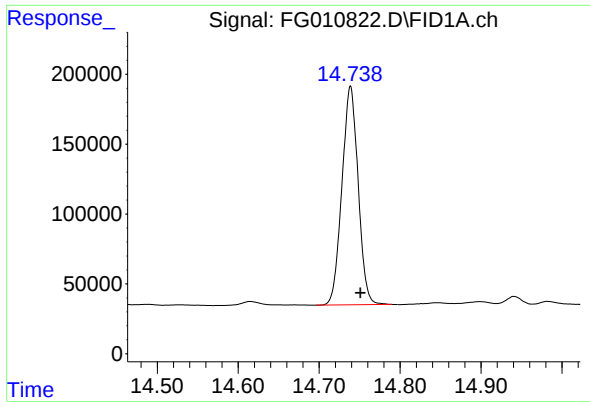

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.739 min
Delta R.T.: -0.012 min
Response: 2175005
Conc: 17.93 ug/ml

Instrument :
FID_G
ClientSampleId :
SASP2-T-3-(10-14)