

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100821\
 Data File : FG008816.D
 Signal(s) : FID1A.ch
 Acq On : 08 Oct 2021 13:55
 Operator : AJ\MA
 Sample : M4089-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 08 23:30:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
 Quant Title :
 QLast Update : Fri Oct 08 03:31:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	2658411	23.031 ug/ml
Target Compounds			
18) N-TETRACONTANE	21.908f	106680	1.198 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100821\
Data File : FG008816.D
Signal(s) : FID1A.ch
Acq On : 08 Oct 2021 13:55
Operator : AJ\MA
Sample : M4089-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 23:30:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

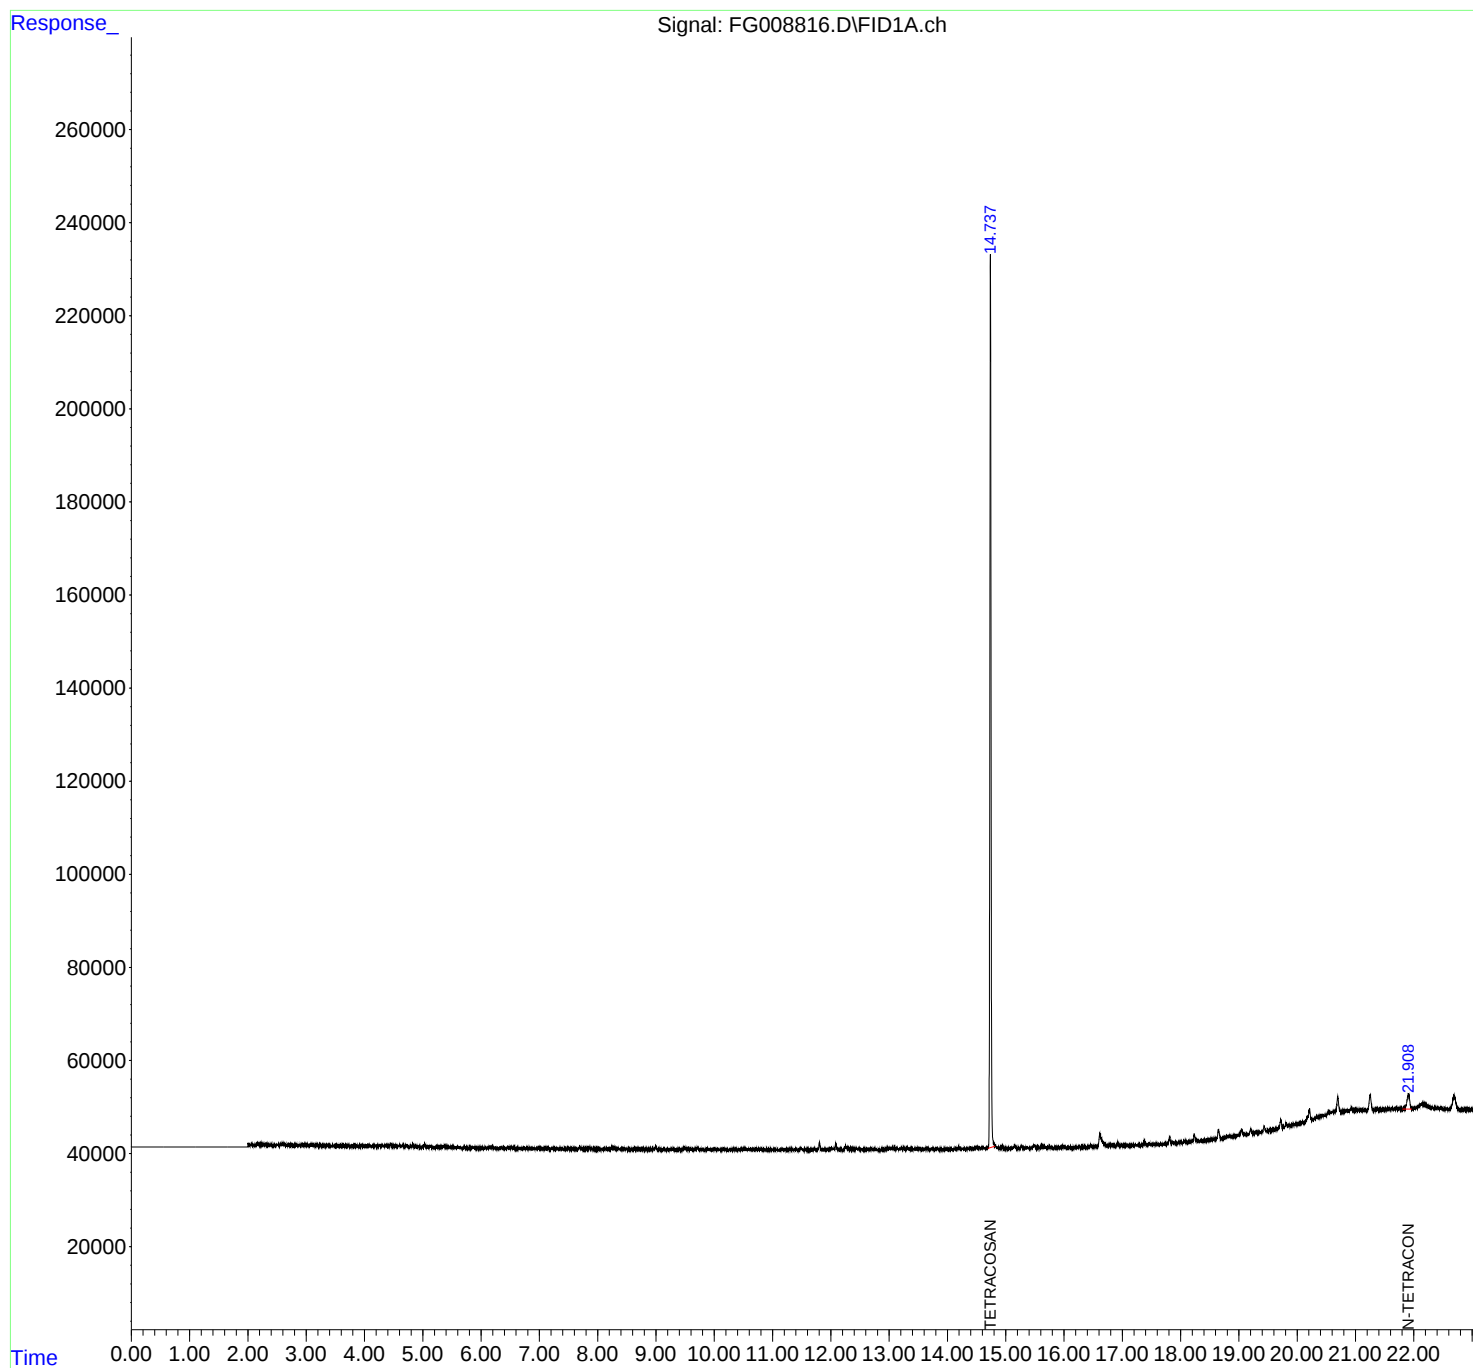


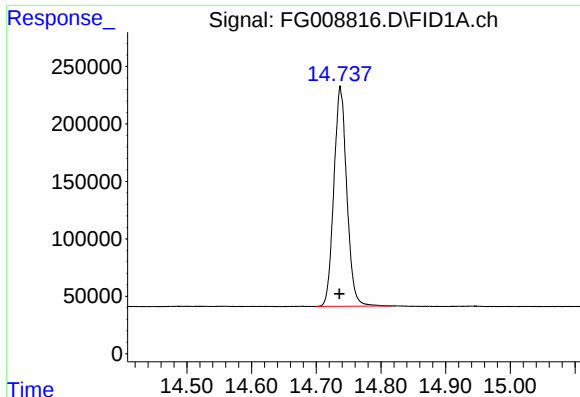

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: 0.001 min
Response: 2658411
Conc: 23.03 ug/ml

Instrument :
FID_G
ClientSampleId :

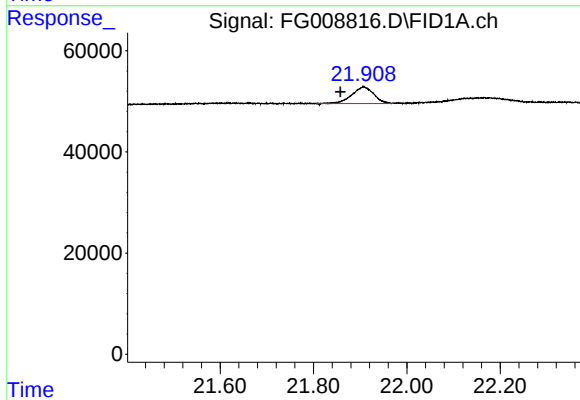

#18 N-TETRACONTANE

R.T.: 21.908 min
Delta R.T.: 0.050 min
Response: 106680
Conc: 1.20 ug/ml