

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100821\
Data File : FG008823.D
Signal(s) : FID1A.ch
Acq On : 08 Oct 2021 17:32
Operator : AJ\MA
Sample : M4119-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 23:32:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	2393677	20.738 ug/ml
Target Compounds			
4) N-TETRADECANE	8.239	117832	0.836 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100821\
Data File : FG008823.D
Signal(s) : FID1A.ch
Acq On : 08 Oct 2021 17:32
Operator : AJ\MA
Sample : M4119-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 23:32:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

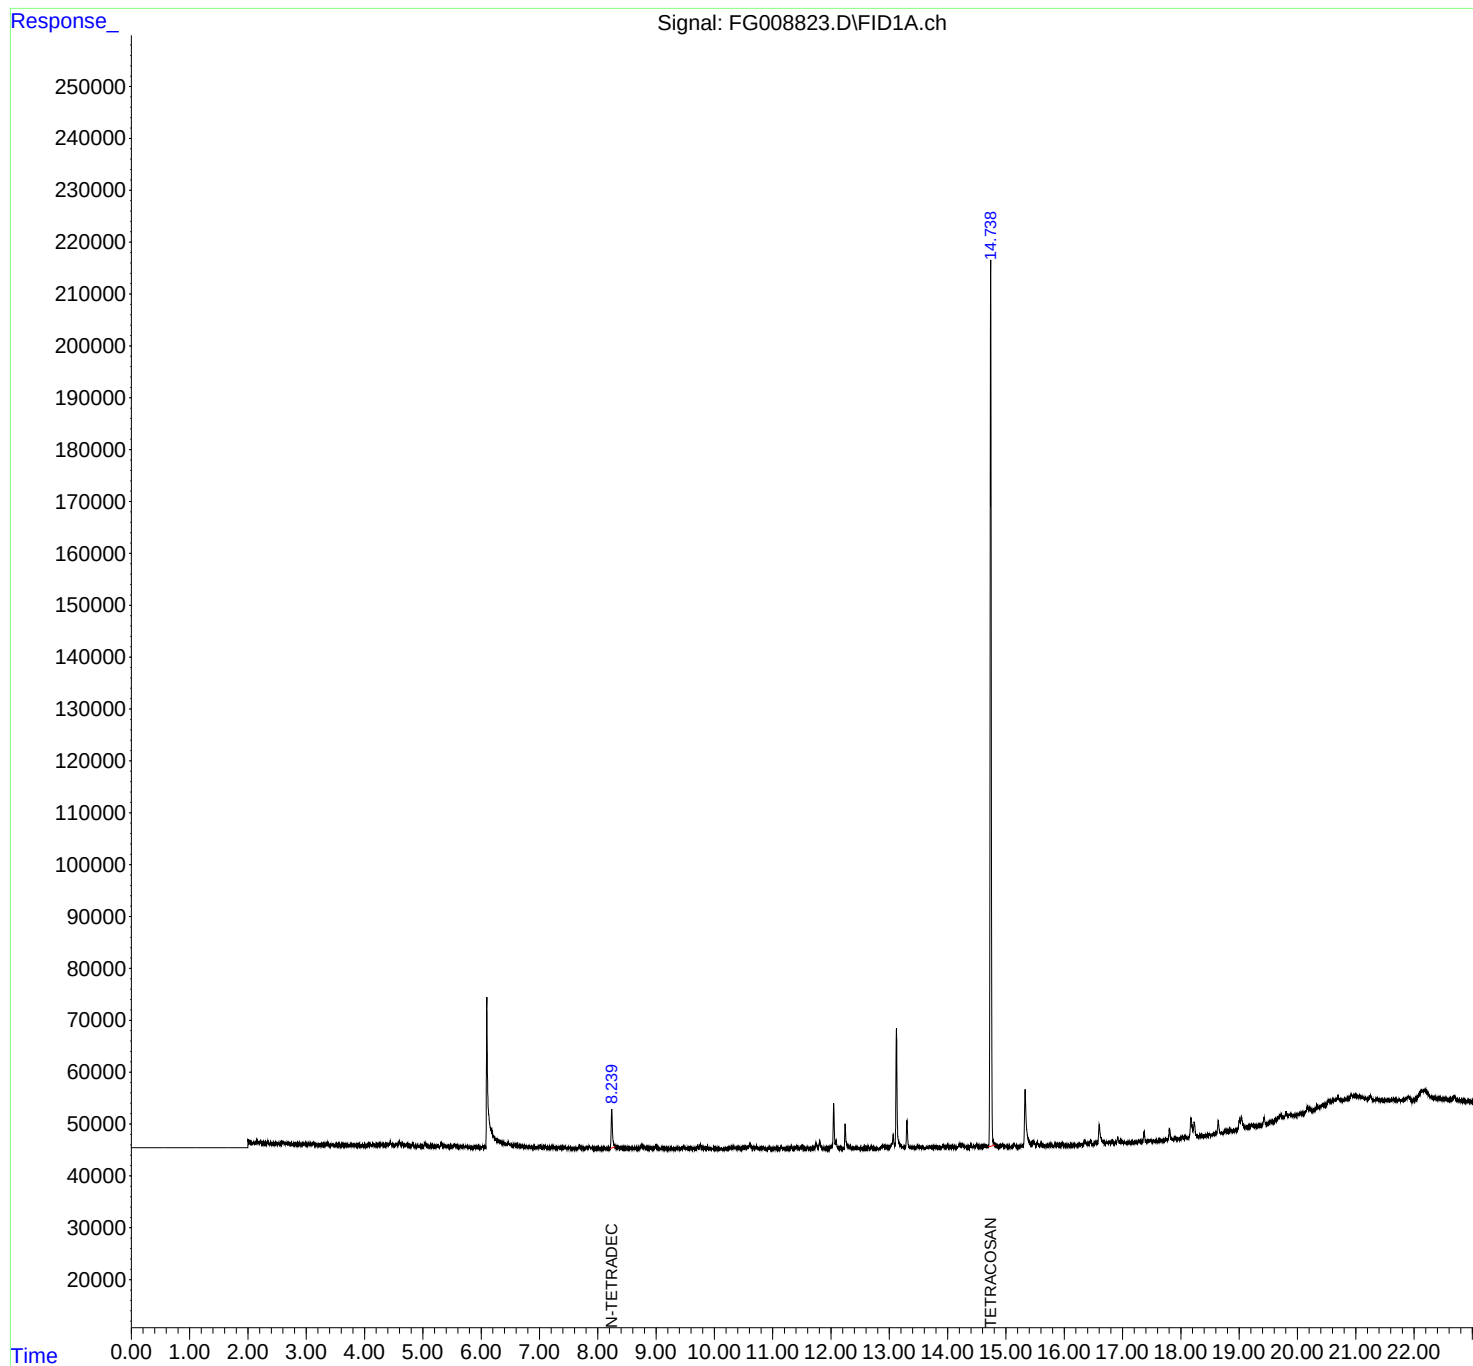


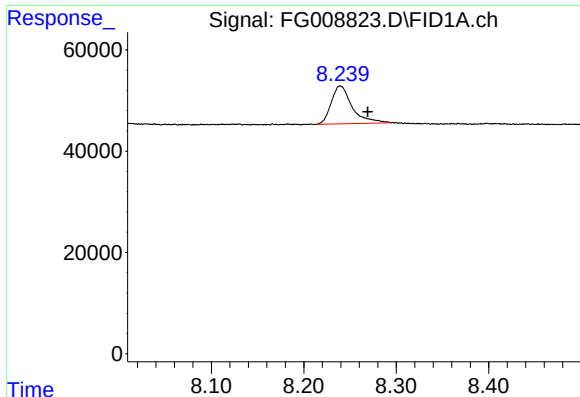

#4 N-TETRADECANE

R.T.: 8.239 min
Delta R.T.: -0.030 min
Response: 117832
Conc: 0.84 ug/ml

Instrument :
FID_G
ClientSampleId :

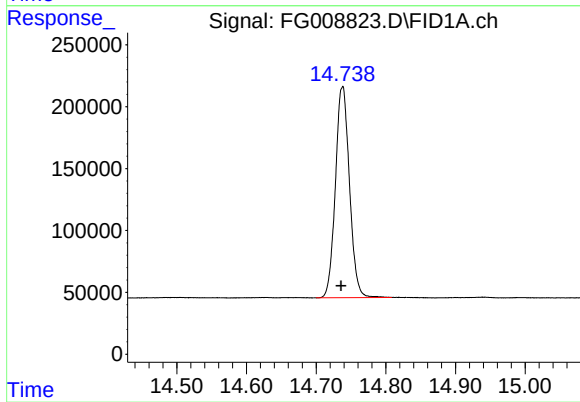

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: 0.002 min
Response: 2393677
Conc: 20.74 ug/ml