

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100923\
Data File : FG013037.D
Signal(s) : FID1A.ch
Acq On : 09 Oct 2023 09:22
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 09 11:17:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092123.M
Quant Title :
QLast Update : Fri Sep 22 02:14:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
15)	N-TETRATRIACONTANE	19.753	153855	1.629 ug/ml
16)	N-HEXATRIACONTANE	20.533	52014	0.704 ug/ml
17)	N-OCTATRIACONTANE	21.306f	75884	1.145 ug/ml
18)	N-TETRACONTANE	22.237	55478	0.880 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100923\
Data File : FG013037.D
Signal(s) : FID1A.ch
Acq On : 09 Oct 2023 09:22
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 09 11:17:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092123.M
Quant Title :
QLast Update : Fri Sep 22 02:14:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

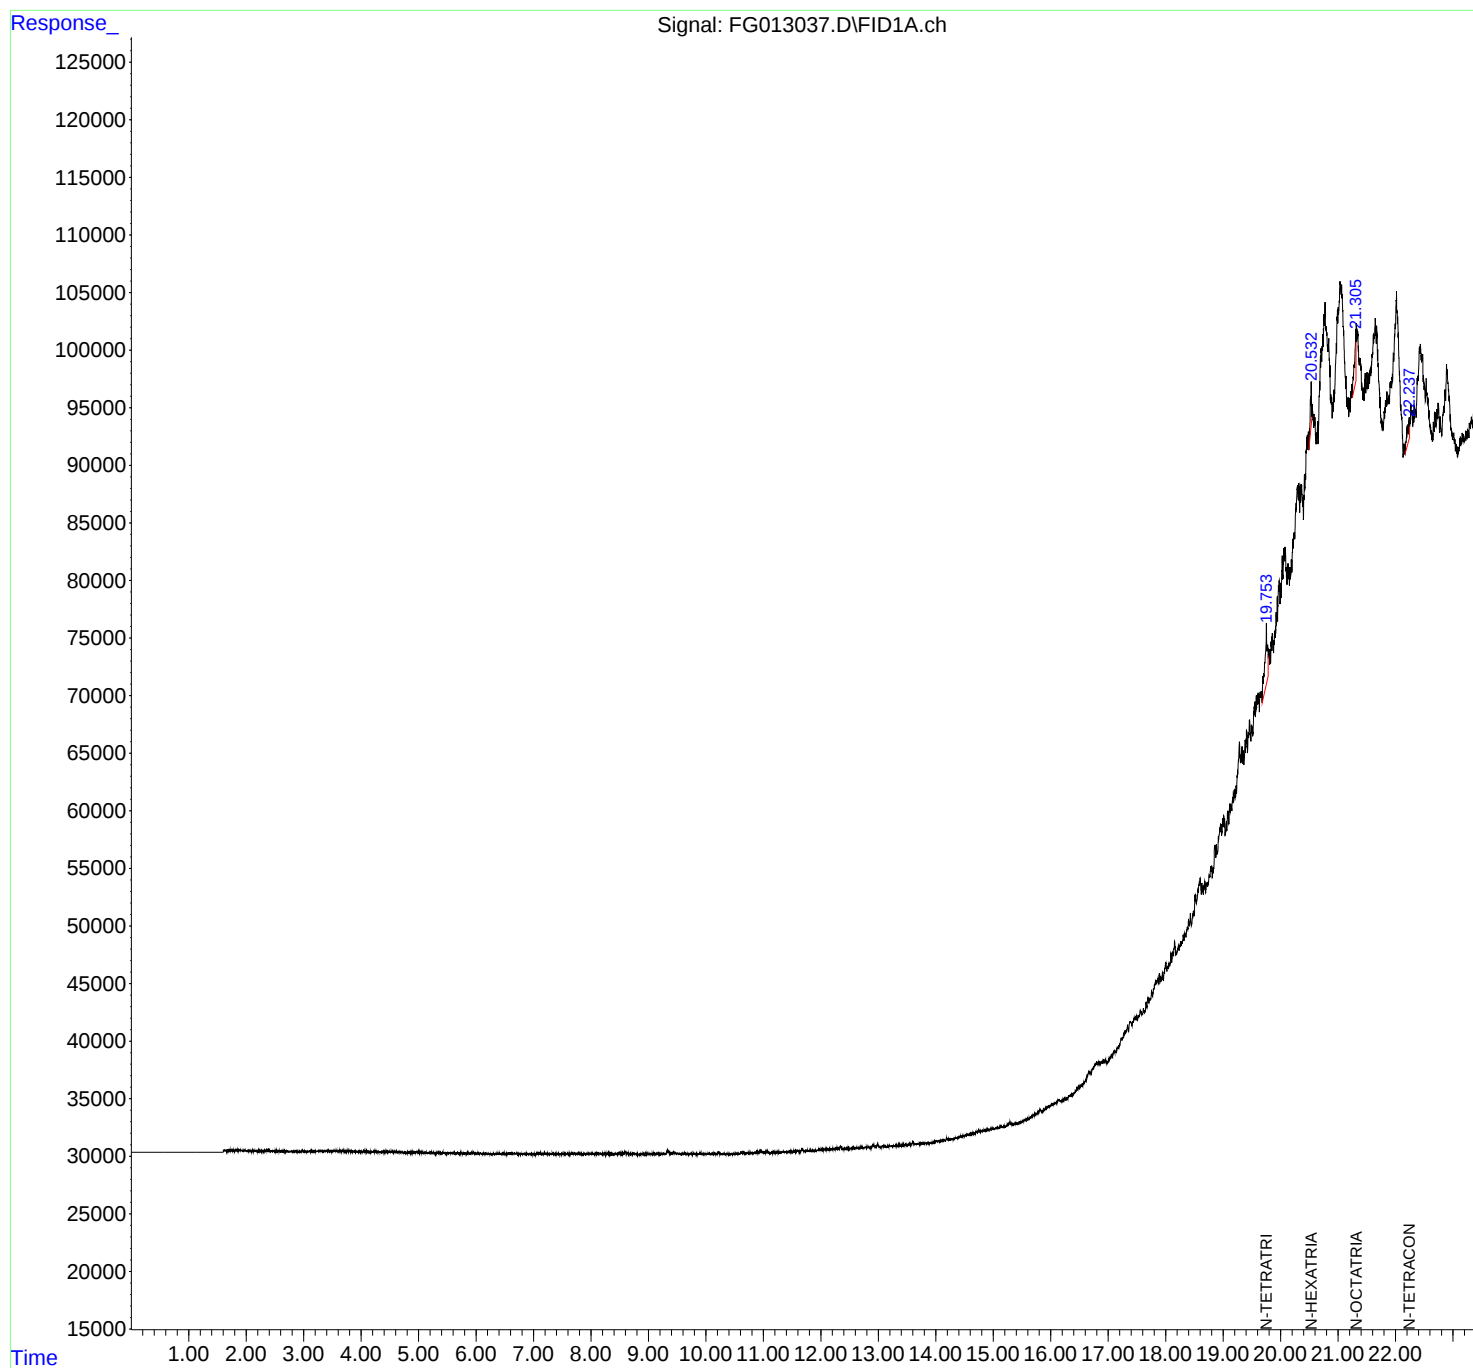


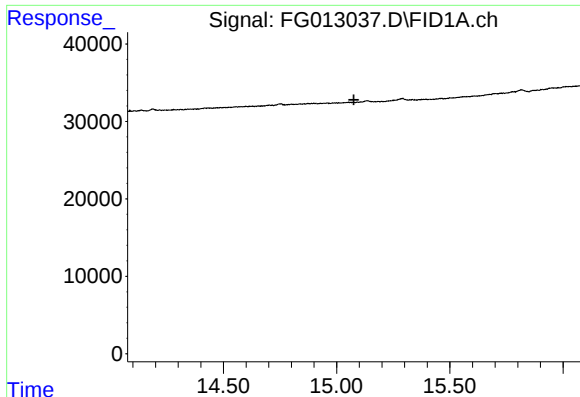

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.076 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

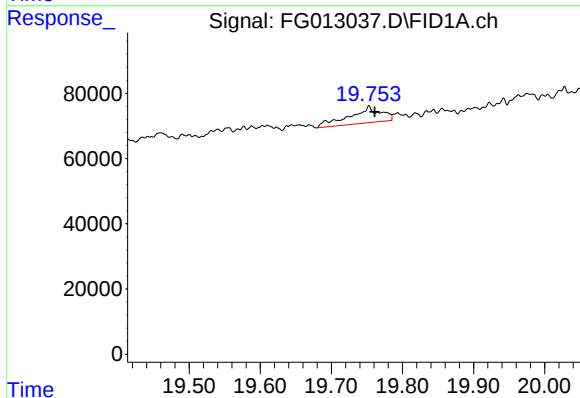


#15 N-TETRATRIACONTANE

R.T.: 19.753 min
Delta R.T.: -0.008 min
Response: 153855
Conc: 1.63 ug/ml

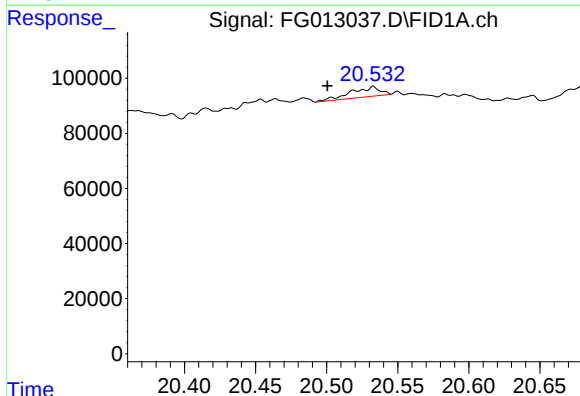


#16 N-HEXATRIACONTANE

R.T.: 20.533 min
Delta R.T.: 0.032 min
Response: 52014
Conc: 0.70 ug/ml

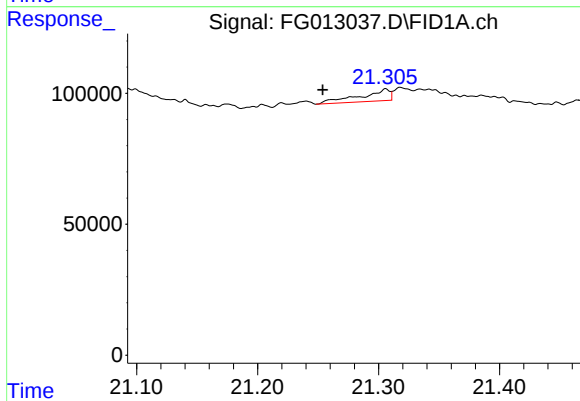

#17 N-OCTATRIACONTANE

R.T.: 21.306 min
Delta R.T.: 0.052 min
Response: 75884
Conc: 1.15 ug/ml

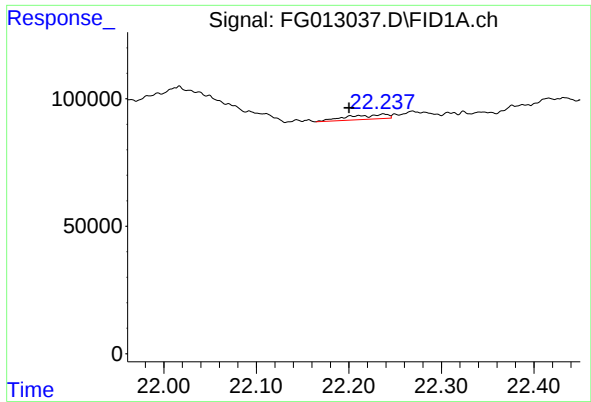

#18 N-TETRACONTANE

R.T.: 22.237 min
Delta R.T.: 0.037 min
Response: 55478
Conc: 0.88 ug/ml

Instrument :
FID_G
ClientSampleId :