

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100923\
Data File : FG013041.D
Signal(s) : FID1A.ch
Acq On : 09 Oct 2023 11:23
Operator : YP\AJ
Sample : 04769-01 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-10-4-2023

Integration File: autoint1.e
Quant Time: Oct 09 12:04:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092123.M
Quant Title :
QLast Update : Fri Sep 22 02:14:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.089	327149	2.887 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100923\
Data File : FG013041.D
Signal(s) : FID1A.ch
Acq On : 09 Oct 2023 11:23
Operator : YP\AJ
Sample : 04769-01 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-10-4-2023

Integration File: autoint1.e
Quant Time: Oct 09 12:04:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092123.M
Quant Title :
QLast Update : Fri Sep 22 02:14:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

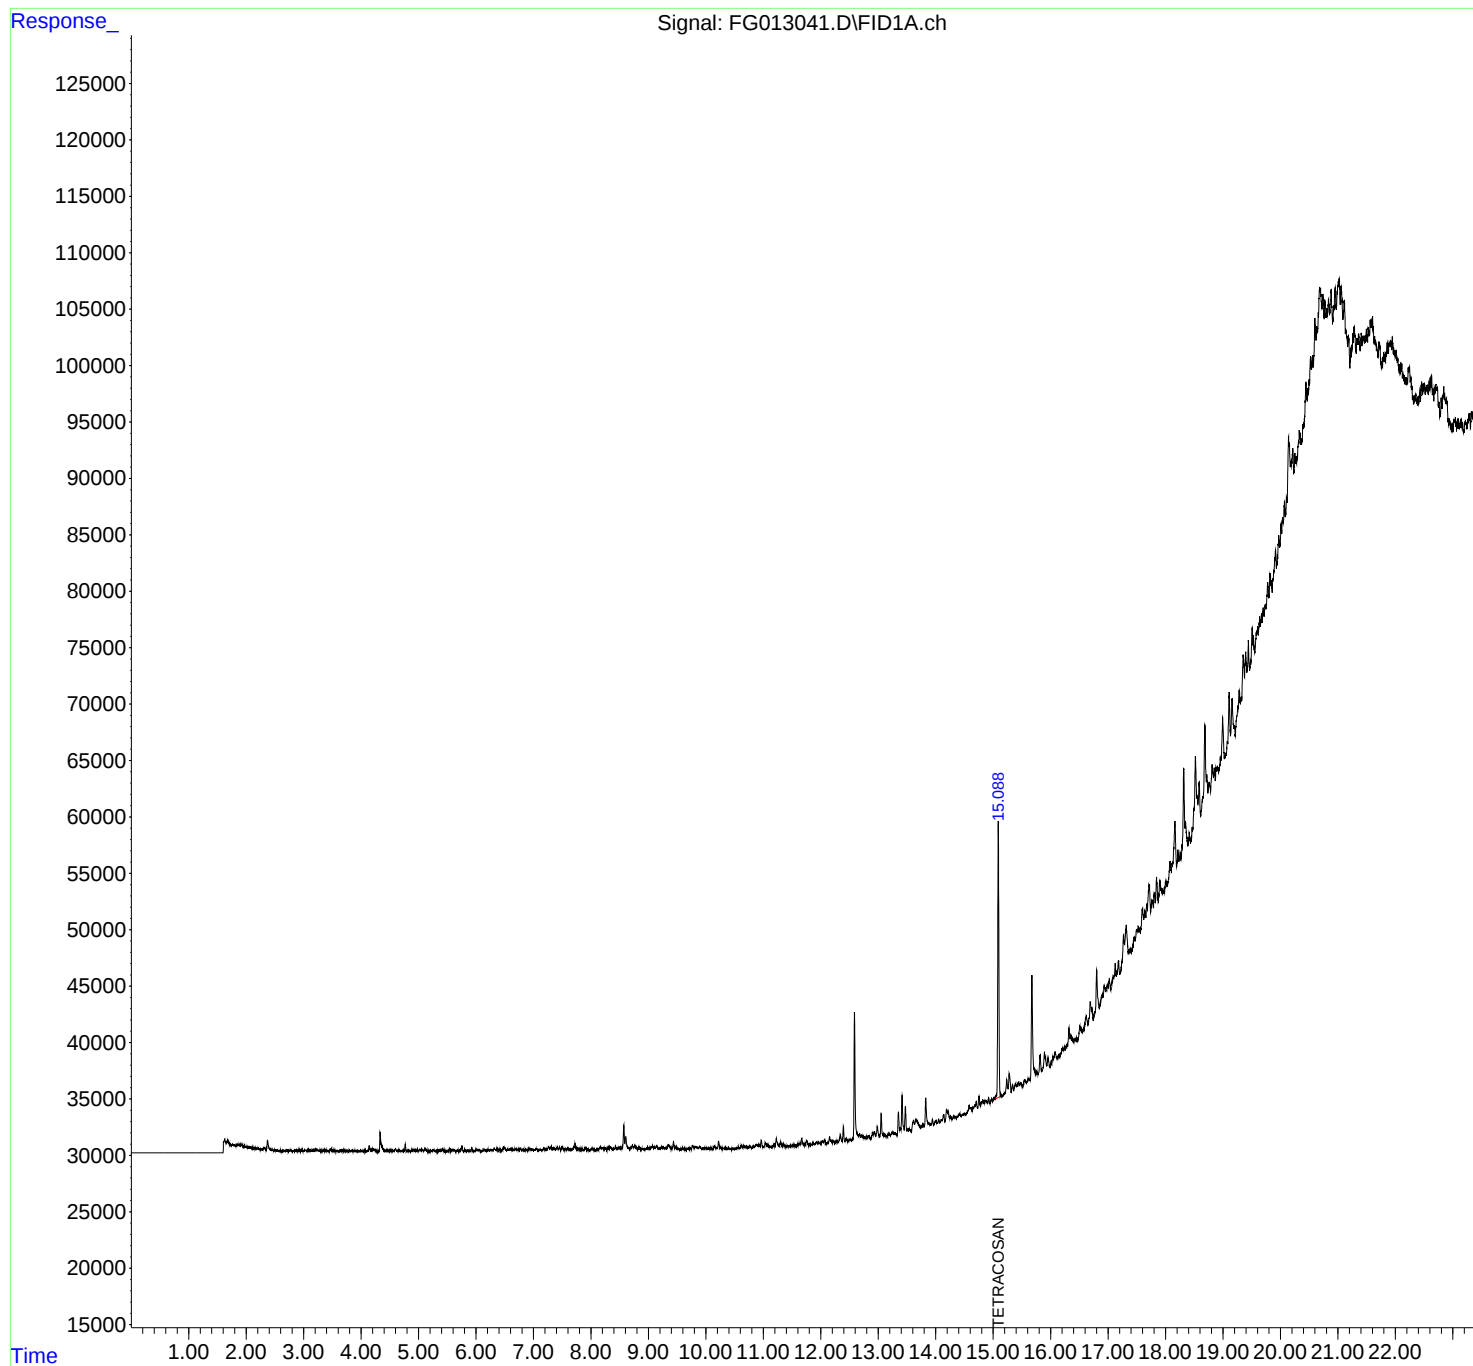

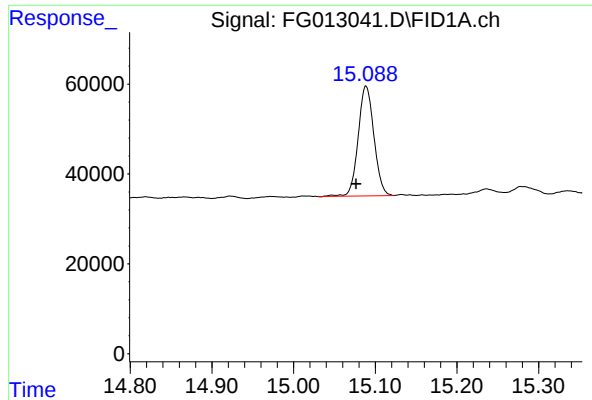

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.089 min
Delta R.T.: 0.012 min
Response: 327149
Conc: 2.89 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-10-4-2023