

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100923AL\
 Data File : FG013047.D
 Signal(s) : FID1A.ch
 Acq On : 09 Oct 2023 14:21
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 09 23:49:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 100623.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 07 07:45:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.997	9697	0.084 ug/ml
19) T n-Tetratriacontane (C34)	19.783	18829	0.168 ug/ml
21) T n-Octatriacontane (C38)	21.297	15993	0.139 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100923AL\
Data File : FG013047.D
Signal(s) : FID1A.ch
Acq On : 09 Oct 2023 14:21
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 09 23:49:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 100623.M
Quant Title : GC Extractables
QLast Update : Sat Oct 07 07:45:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

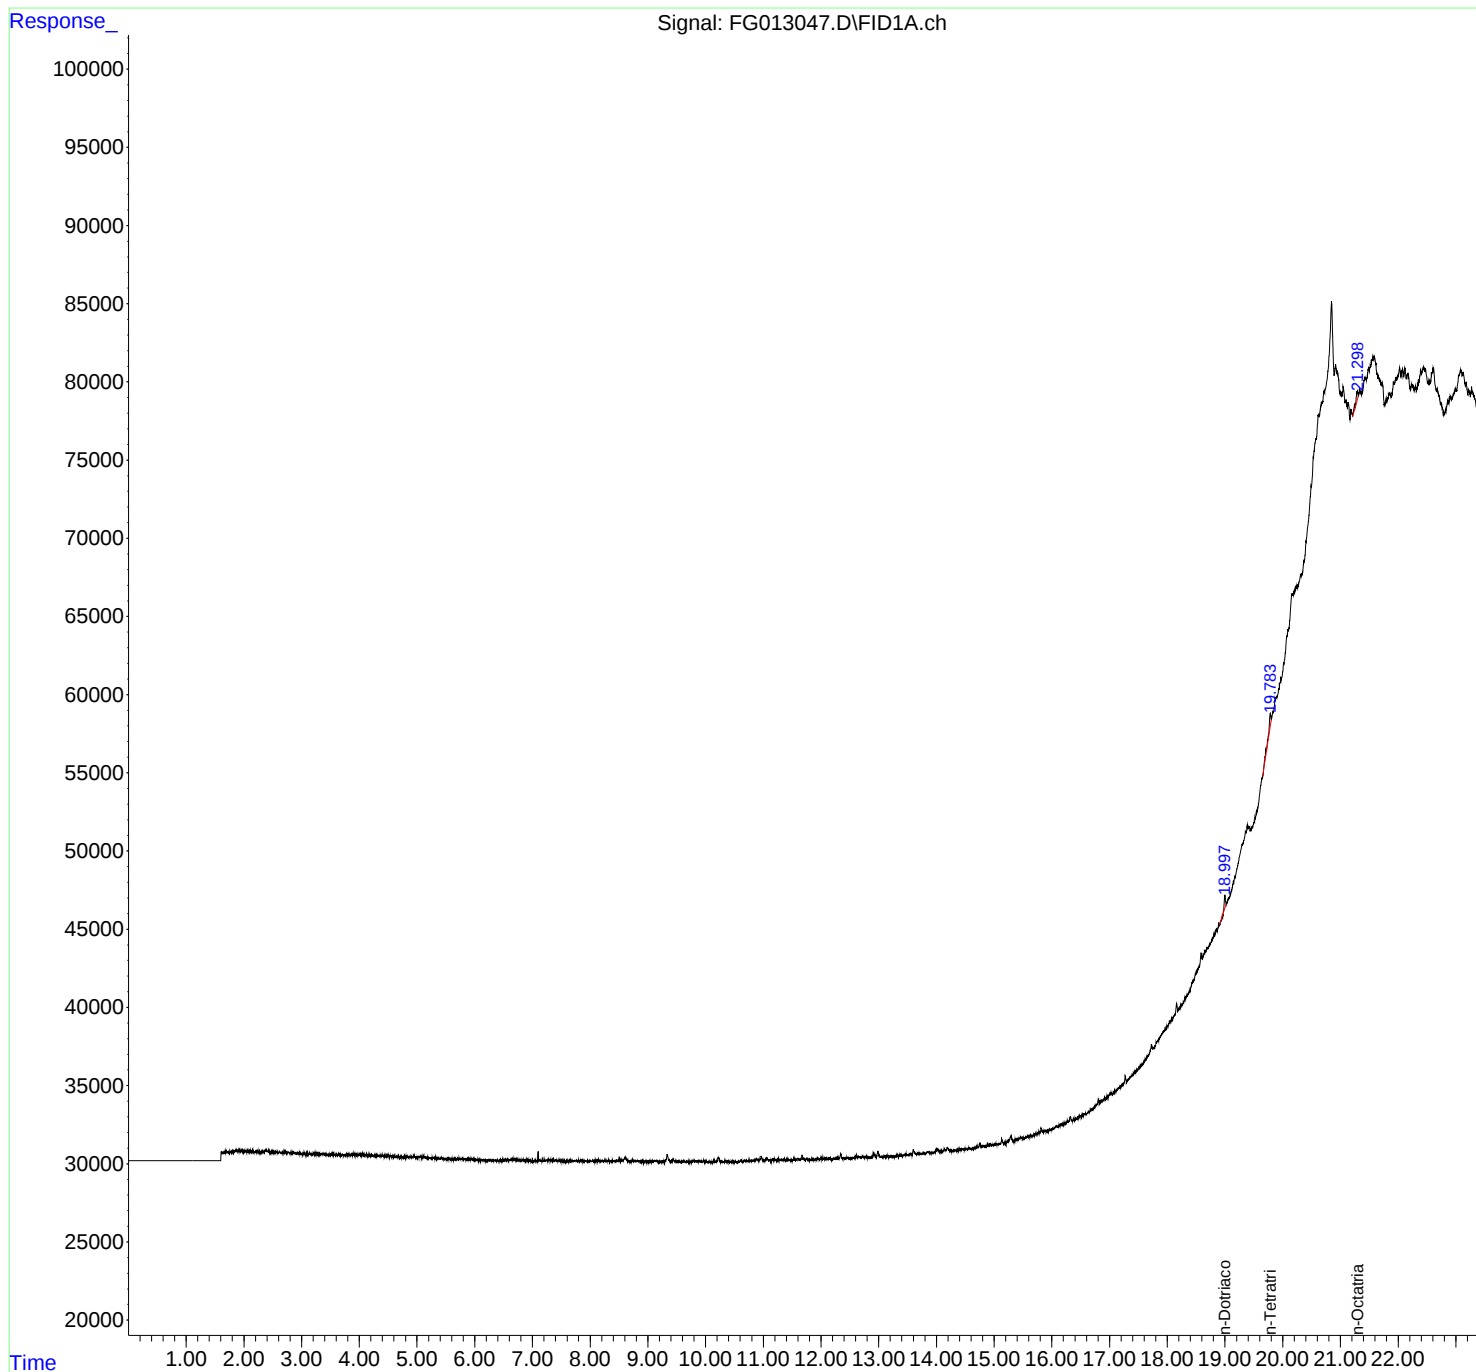


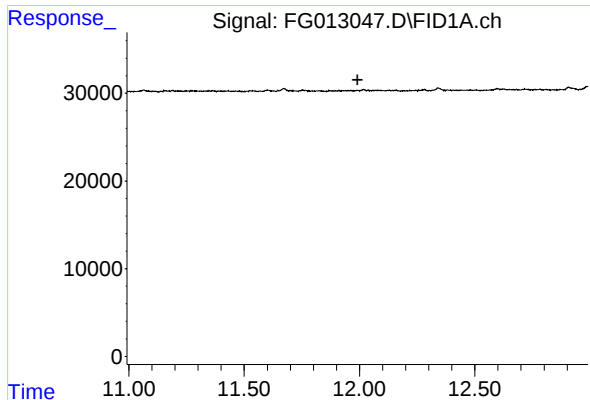

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.991 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

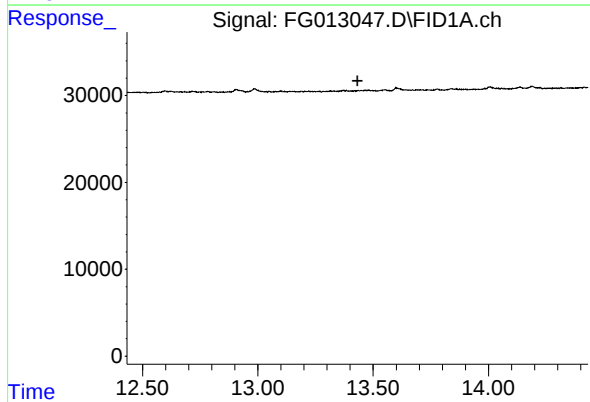


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.432 min
Response: 0
Conc: N.D.

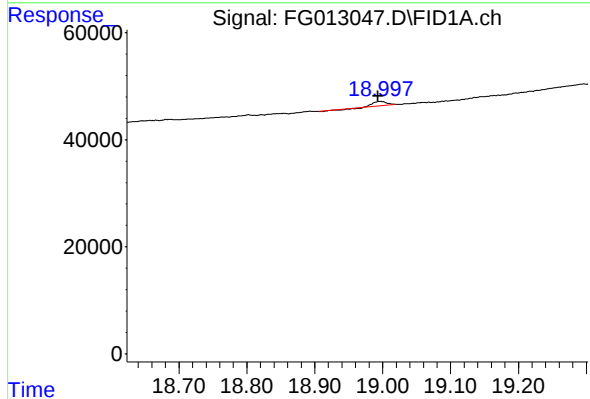


#18 n-Dotriacontane (C32)

R.T.: 18.997 min
Delta R.T.: 0.004 min
Response: 9697
Conc: 0.08 ug/ml

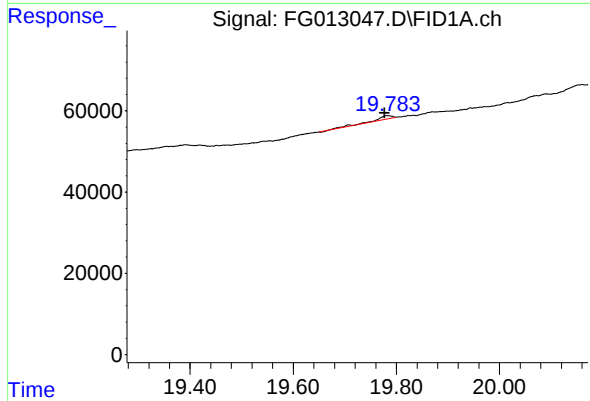

#19 n-Tetratriacontane (C34)

R.T.: 19.783 min
Delta R.T.: 0.006 min
Response: 18829
Conc: 0.17 ug/ml

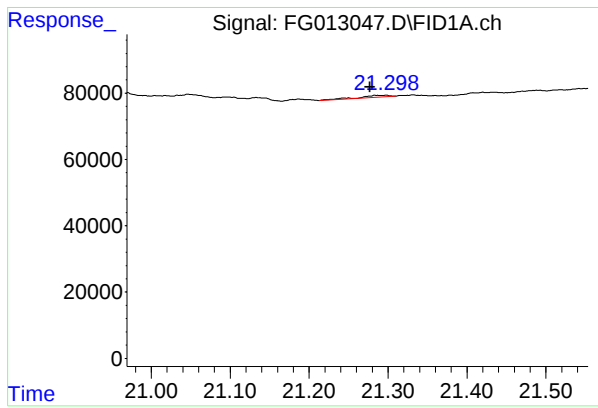

#21 n-Octatriacontane (C38)

R.T.: 21.297 min
Delta R.T.: 0.021 min
Response: 15993
Conc: 0.14 ug/ml

Instrument :

FID_G

ClientSampleId :