

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101023AL\
Data File : FG013060.D
Signal(s) : FID1A.ch
Acq On : 10 Oct 2023 08:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 00:10:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 100623.M
Quant Title : GC Extractables
QLast Update : Sat Oct 07 07:45:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.771	10293	0.092 ug/ml
20) T	n-Hexatriacontane (C36)	20.562	92549	0.812 ug/ml
21) T	n-Octatriacontane (C38)	21.328f	14148	0.123 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101023AL\
Data File : FG013060.D
Signal(s) : FID1A.ch
Acq On : 10 Oct 2023 08:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 00:10:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 100623.M
Quant Title : GC Extractables
QLast Update : Sat Oct 07 07:45:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

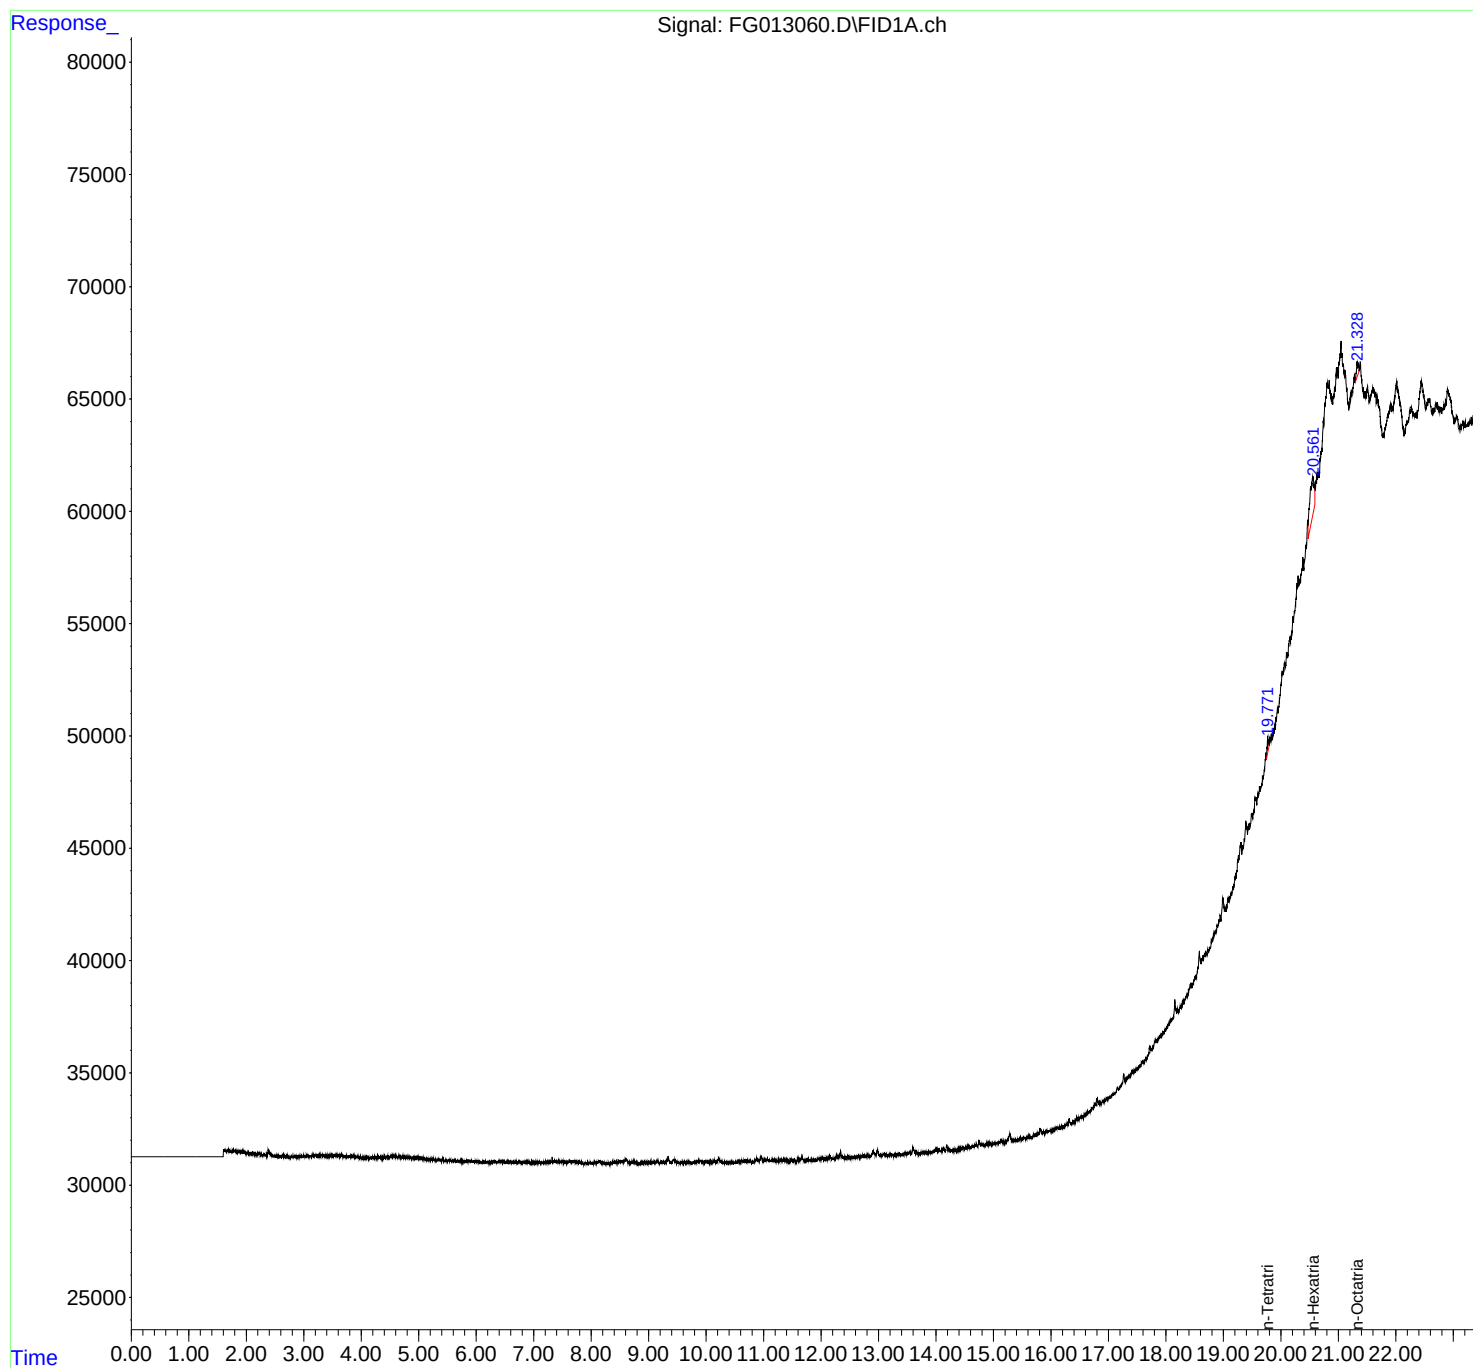


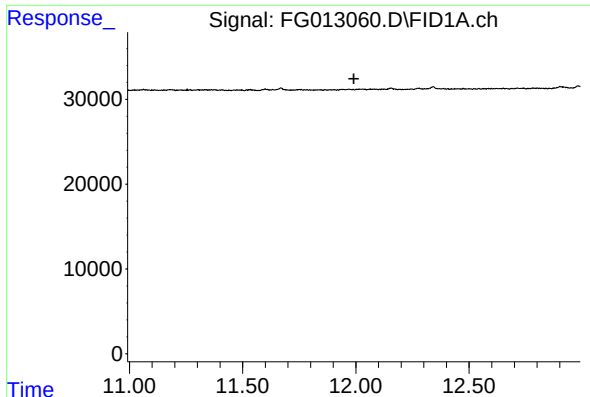

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.991 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

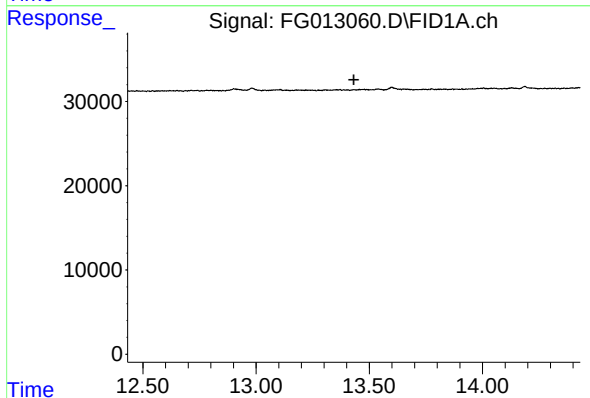


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.432 min
Response: 0
Conc: N.D.

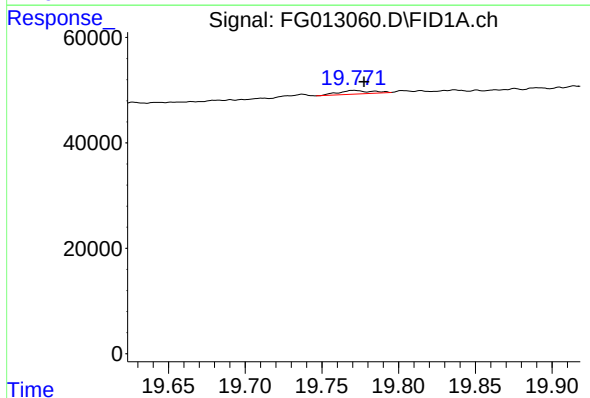


#19 n-Tetratriacontane (C34)

R.T.: 19.771 min
Delta R.T.: -0.007 min
Response: 10293
Conc: 0.09 ug/ml

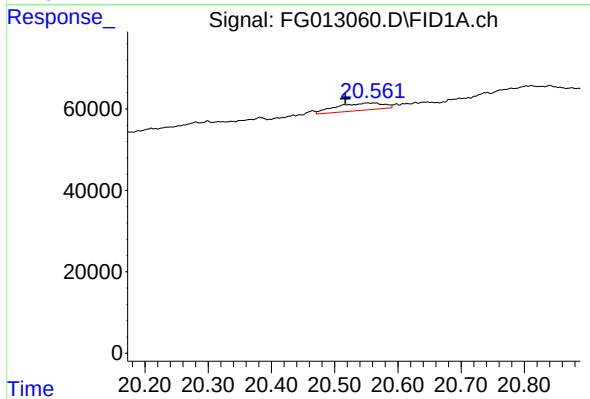

#20 n-Hexatriacontane (C36)

R.T.: 20.562 min
Delta R.T.: 0.045 min
Response: 92549
Conc: 0.81 ug/ml

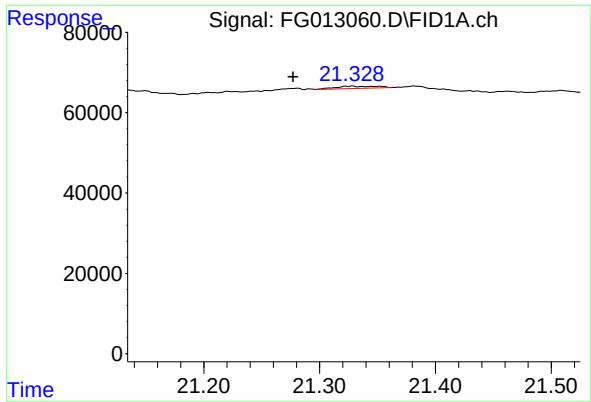

#21 n-Octatriacontane (C38)

R.T.: 21.328 min
Delta R.T.: 0.051 min
Response: 14148
Conc: 0.12 ug/ml

Instrument :
FID_G
ClientSampleId :