

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101023AL\
 Data File : FG013063.D
 Signal(s) : FID1A.ch
 Acq On : 10 Oct 2023 10:05
 Operator : YP\AJ
 Sample : PB156129BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 11 00:13:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 100623.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 07 07:45:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.432	4030215	39.991 ug/ml
Spiked Amount 50.000		Recovery =	79.98%
Target Compounds			
4) T n-Dodecane (C12)	6.770	69342	0.569 ug/ml
6) T n-Tetradecane (C14)	8.604	41338	0.346 ug/ml
7) T n-Hexadecane (C16)	10.220	21779	0.178 ug/ml
8) T n-Octadecane (C18)	11.667	22499	0.184 ug/ml
10) T n-Eicosane (C20)	12.981	20580	0.176 ug/ml
17) T n-Tricontane (C30)	18.155	26922	0.235 ug/ml
18) T n-Dotriacontane (C32)	18.990	38647	0.337 ug/ml
19) T n-Tetratriacontane (C34)	19.775	29026	0.259 ug/ml
20) T n-Hexatriacontane (C36)	20.515	21384	0.188 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101023AL\
Data File : FG013063.D
Signal(s) : FID1A.ch
Acq On : 10 Oct 2023 10:05
Operator : YP\AJ
Sample : PB156129BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 00:13:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 100623.M
Quant Title : GC Extractables
QLast Update : Sat Oct 07 07:45:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

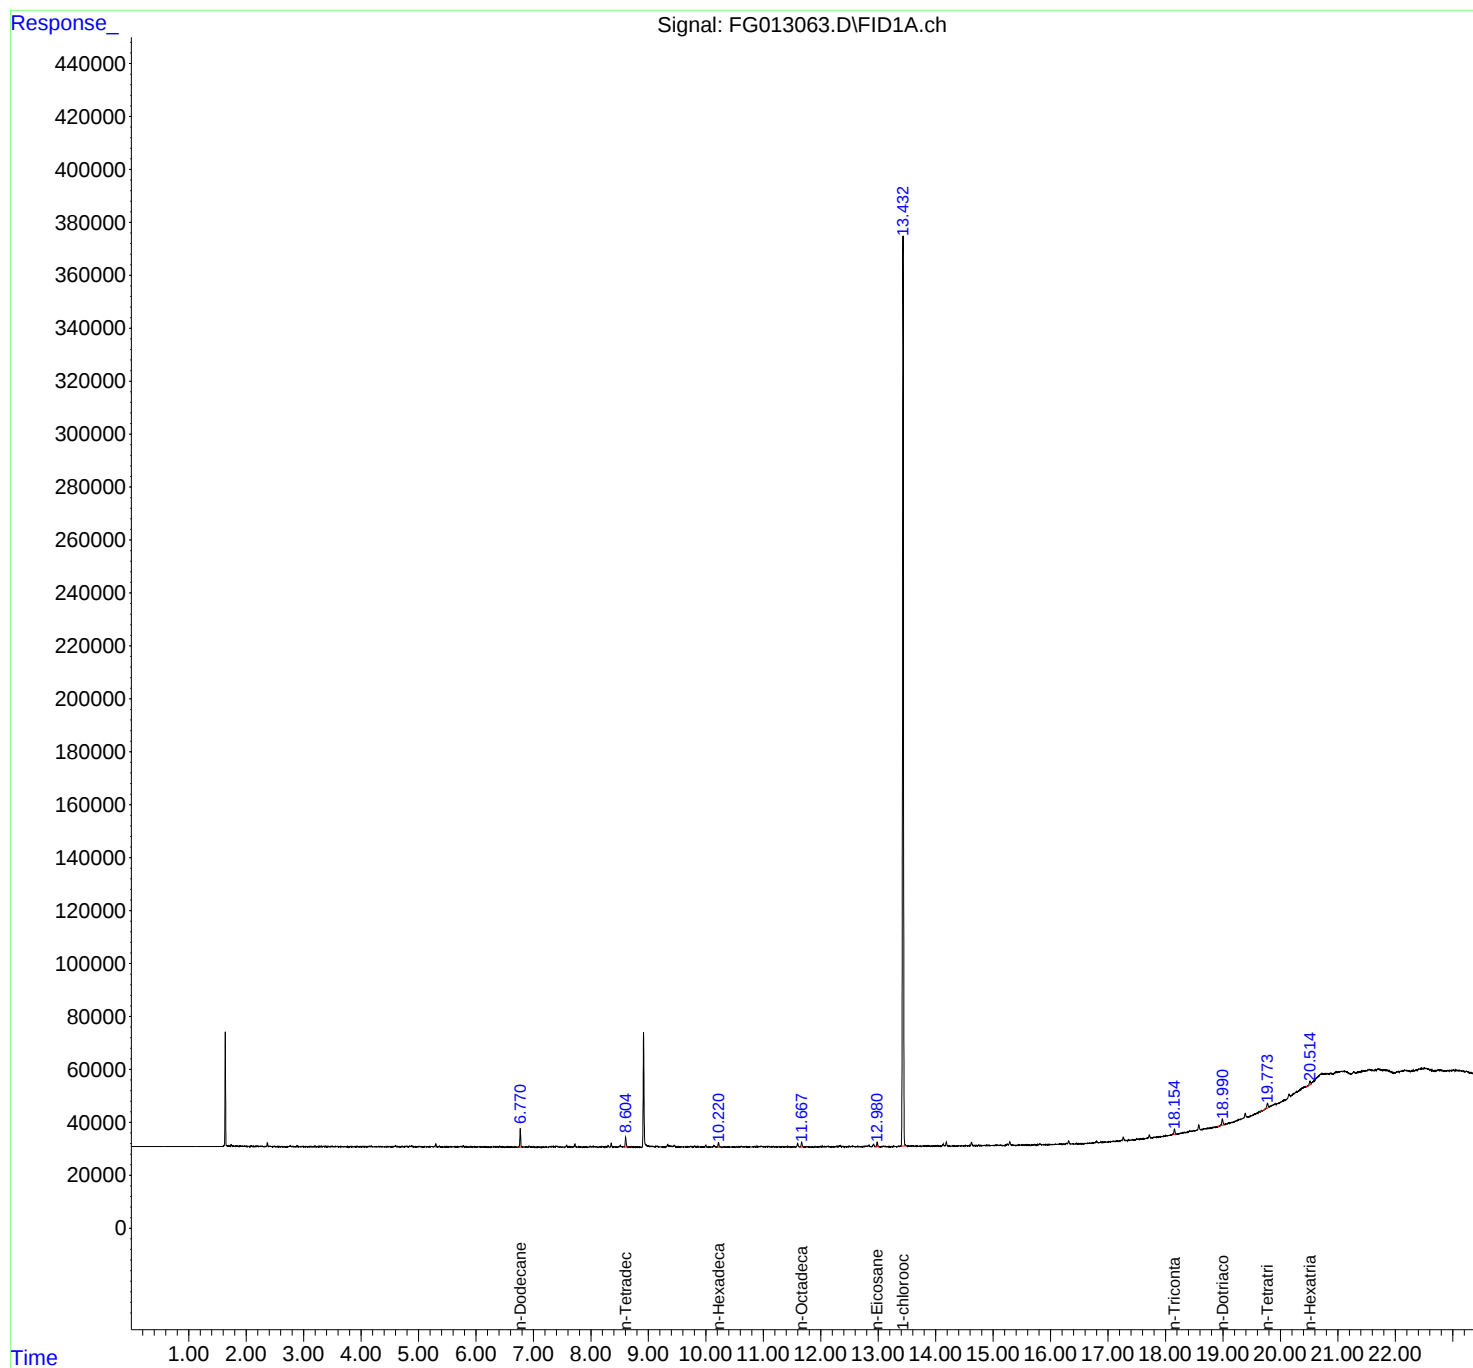


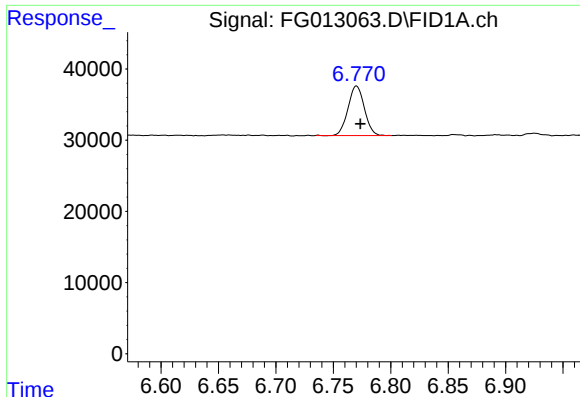

#4 n-Dodecane (C12)


R.T.: 6.770 min
Delta R.T.: -0.003 min
Response: 69342
Conc: 0.57 ug/ml

Instrument :
FID_G
ClientSampleId :

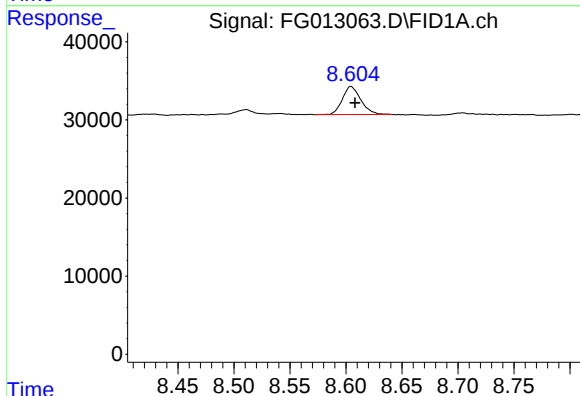


#6 n-Tetradecane (C14)

R.T.: 8.604 min
Delta R.T.: -0.004 min
Response: 41338
Conc: 0.35 ug/ml

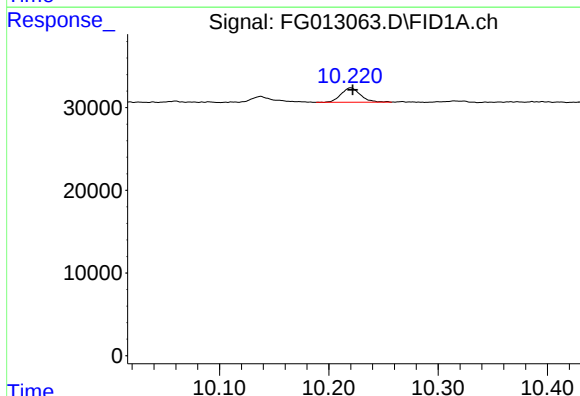


#7 n-Hexadecane (C16)

R.T.: 10.220 min
Delta R.T.: -0.002 min
Response: 21779
Conc: 0.18 ug/ml

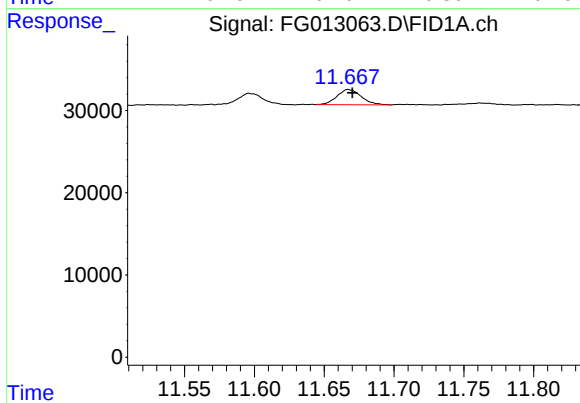

#8 n-Octadecane (C18)


R.T.: 11.667 min
Delta R.T.: -0.003 min
Response: 22499
Conc: 0.18 ug/ml

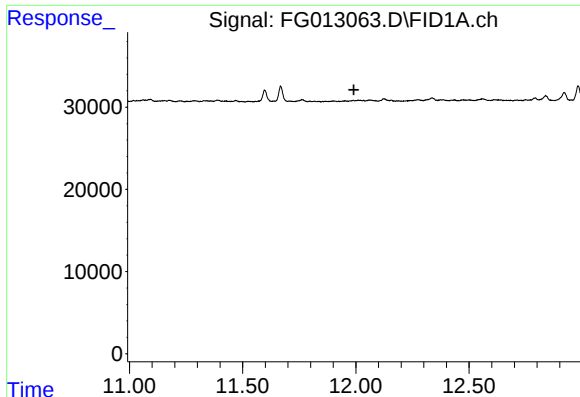

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.991 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

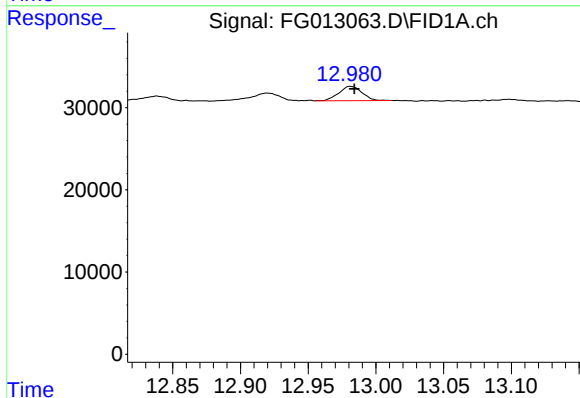


#10 n-Eicosane (C20)

R.T.: 12.981 min
Delta R.T.: -0.003 min
Response: 20580
Conc: 0.18 ug/ml

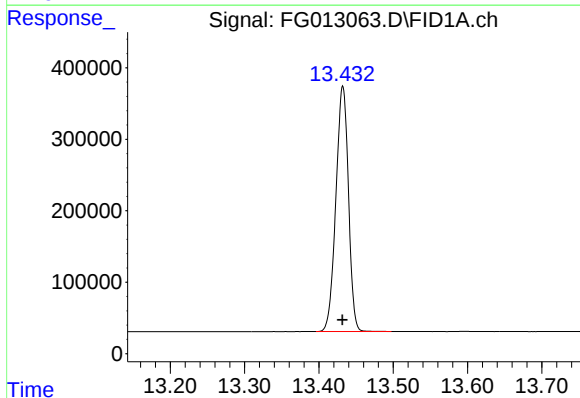


#12 1-chlorooctadecane (SURR)

R.T.: 13.432 min
Delta R.T.: 0.000 min
Response: 4030215
Conc: 39.99 ug/ml

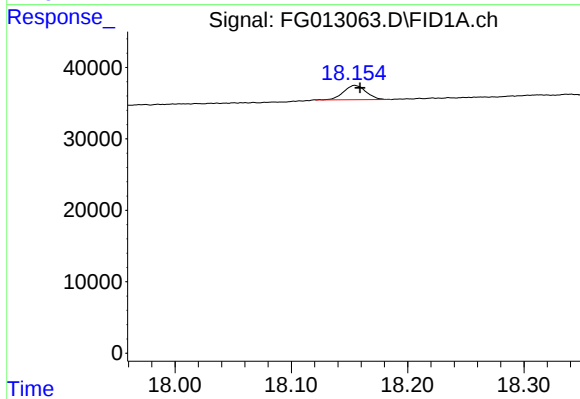

#17 n-Tricontane (C30)


R.T.: 18.155 min
Delta R.T.: -0.004 min
Response: 26922
Conc: 0.24 ug/ml

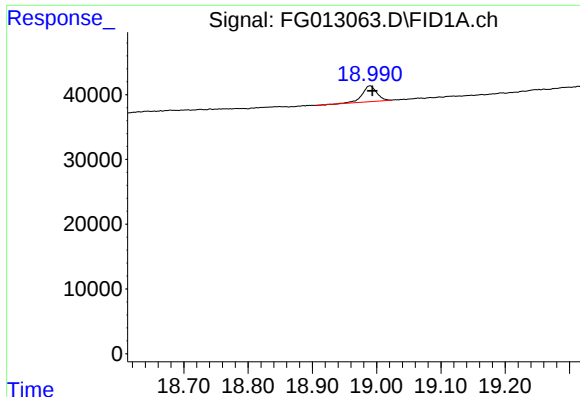

#18 n-Dotriacontane (C32)


R.T.: 18.990 min
Delta R.T.: -0.004 min
Response: 38647
Conc: 0.34 ug/ml

Instrument :
FID_G
ClientSampleId :

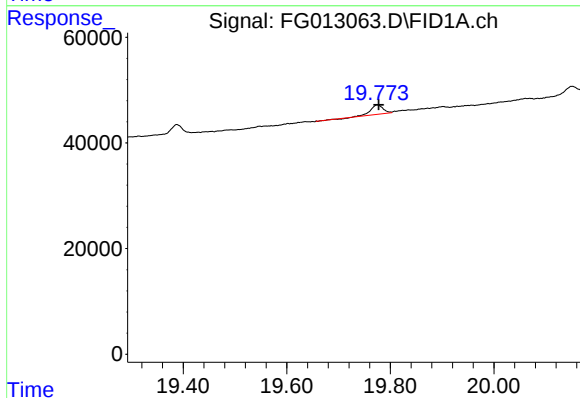

#19 n-Tetratriacontane (C34)

R.T.: 19.775 min
Delta R.T.: -0.003 min
Response: 29026
Conc: 0.26 ug/ml

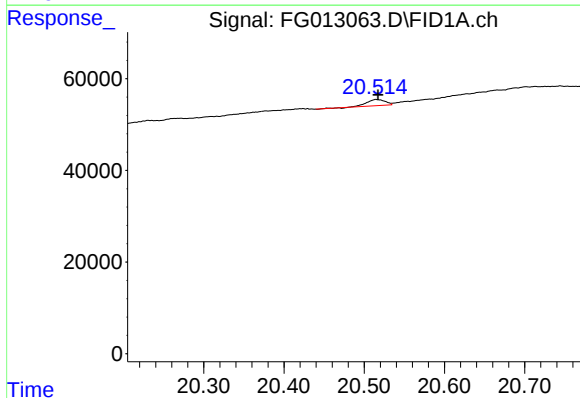

#20 n-Hexatriacontane (C36)

R.T.: 20.515 min
Delta R.T.: -0.003 min
Response: 21384
Conc: 0.19 ug/ml