

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG101121\  
 Data File : FG008832.D  
 Signal(s) : FID1A.ch  
 Acq On : 11 Oct 2021 12:33  
 Operator : AJ\MA  
 Sample : M4146-01  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :  
 20-SB-3-20211007-5.0-5.5

Manual Integrations  
 APPROVED

Sohil  
 10/22/2021 11:13:19 AM

Integration File: autoint1.e  
 Quant Time: Oct 12 01:49:54 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG100721.M  
 Quant Title :  
 QLast Update : Fri Oct 08 03:31:08 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.735 | 2495023  | 21.616 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG101121\  
Data File : FG008832.D  
Signal(s) : FID1A.ch  
Acq On : 11 Oct 2021 12:33  
Operator : AJ\MA  
Sample : M4146-01  
Misc :  
ALS Vial : 7 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
20-SB-3-20211007-5.0-5.5


Manual Integrations  
APPROVED

Sohil  
10/22/2021 11:13:19 AM

Integration File: autoint1.e  
Quant Time: Oct 12 01:49:54 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG100721.M  
Quant Title :  
QLast Update : Fri Oct 08 03:31:08 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

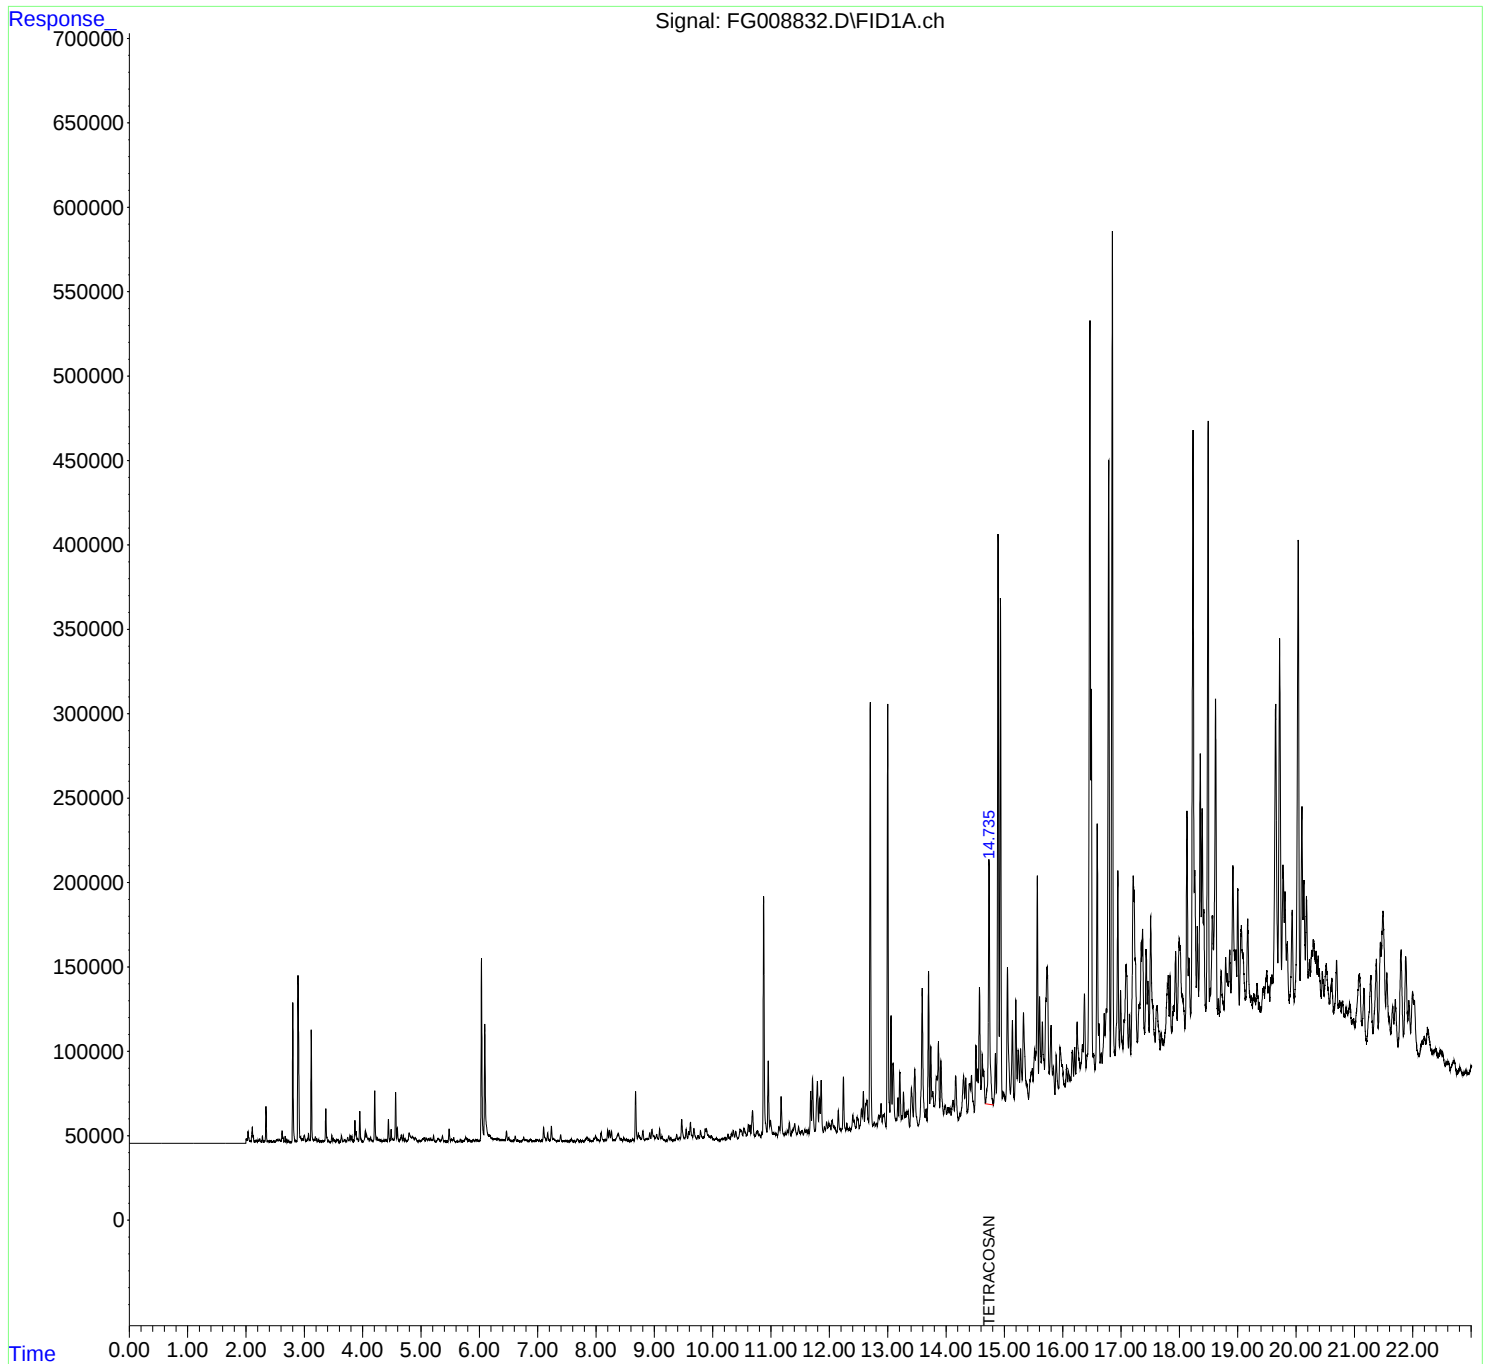

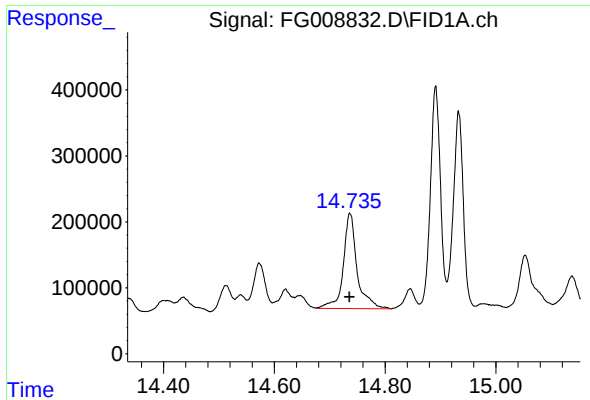

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.735 min  
Delta R.T.: 0.000 min  
Response: 2495023  
Conc: 21.62 ug/ml m

Instrument :  
FID\_G  
ClientSampleId :  
20-SB-3-20211007-5.0-5.5

Manual Integrations  
APPROVED

Sohil  
10/22/2021 11:13:19 AM