

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101122\
 Data File : FG010842.D
 Signal(s) : FID1A.ch
 Acq On : 11 Oct 2022 17:56
 Operator : YP\AJ
 Sample : N5066-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 12 07:50:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
 Quant Title :
 QLast Update : Thu Sep 29 02:21:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	4364918	35.979 ug/ml
Target Compounds			
7) N-EICOSANE	12.645	1086491	7.683 ug/ml
8) N-DOCOSANE	13.840	5866770	42.380 ug/ml
10) N-TETRACOSANE	14.952	9724715	70.585 ug/ml
11) N-HEXACOSANE	15.973	7903434	58.582 ug/ml
12) N-OCTACOSANE	16.920	4956162	37.795 ug/ml
13) N-TRIACONTANE	17.807	2379629	18.487 ug/ml
14) N-DOTRIACONTANE	18.638	1383244	10.885 ug/ml
15) N-TETRATRIACONTANE	19.421	399488	3.182 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101122\
Data File : FG010842.D
Signal(s) : FID1A.ch
Acq On : 11 Oct 2022 17:56
Operator : YP\AJ
Sample : N5066-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 12 07:50:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

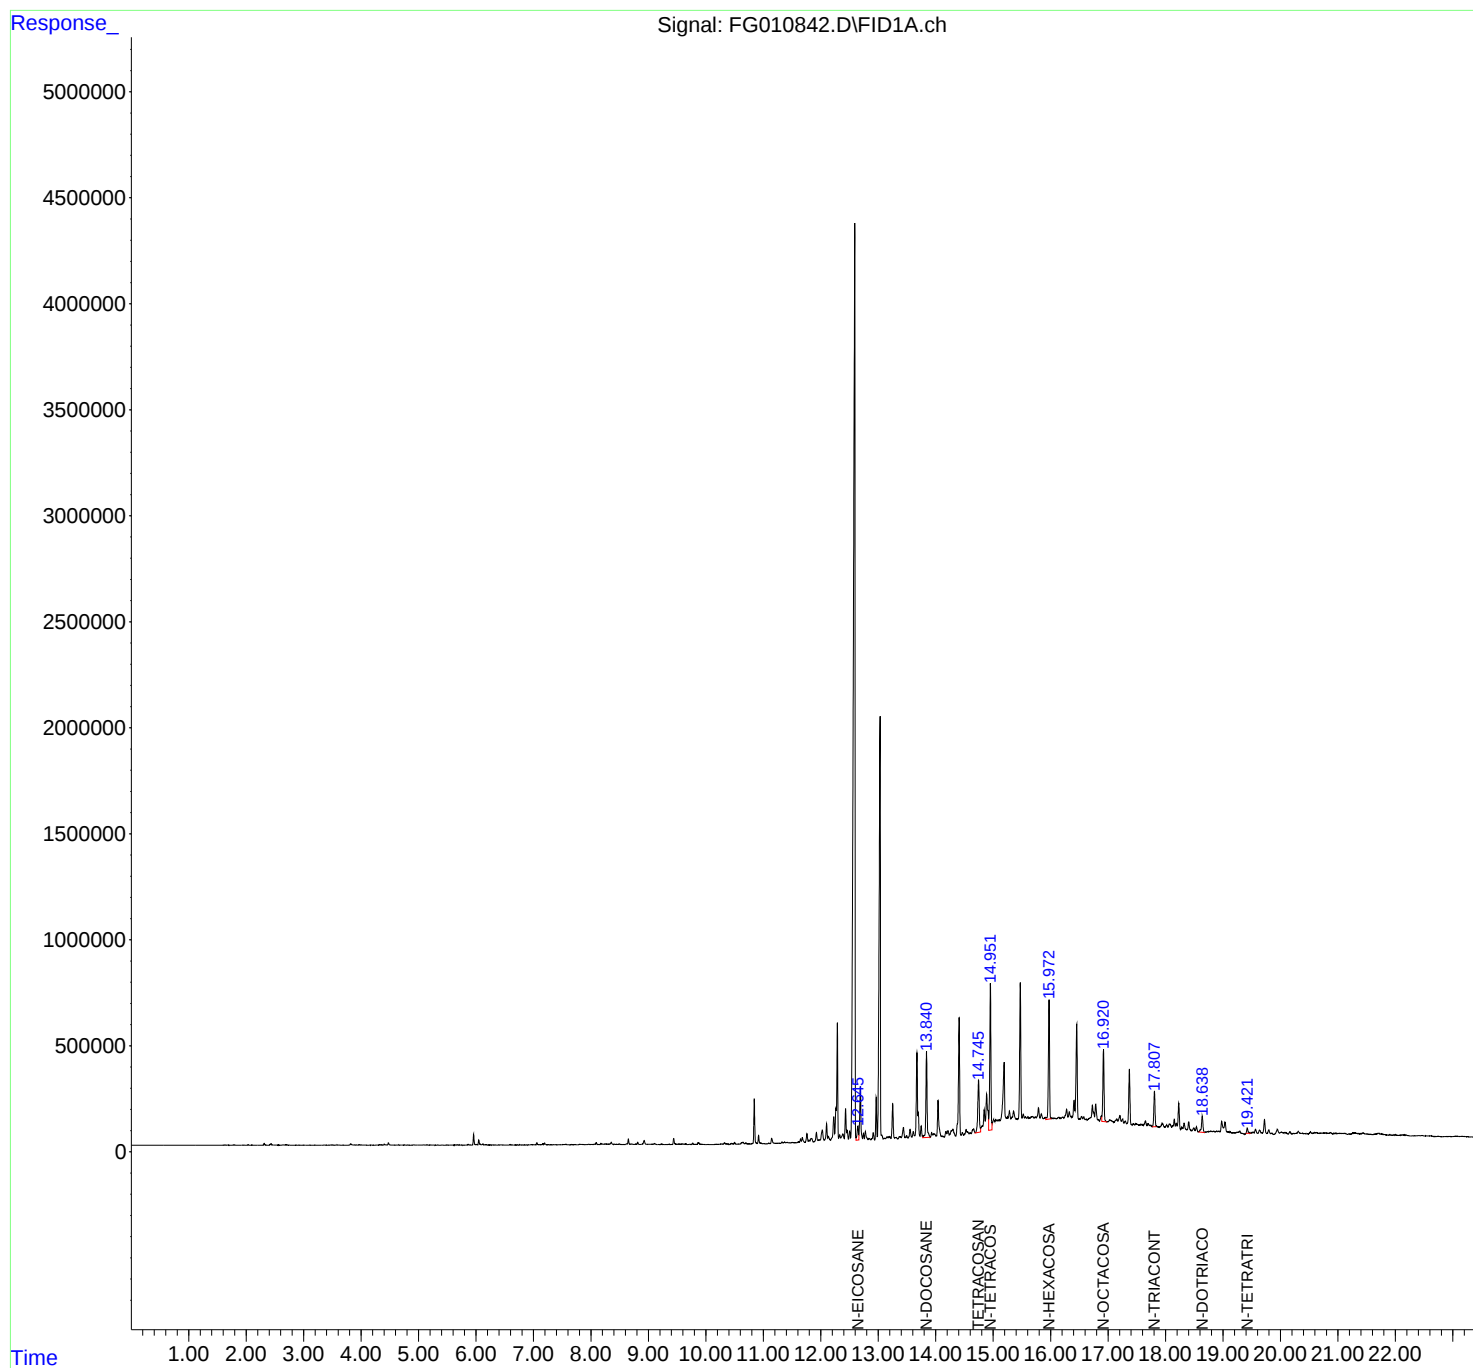


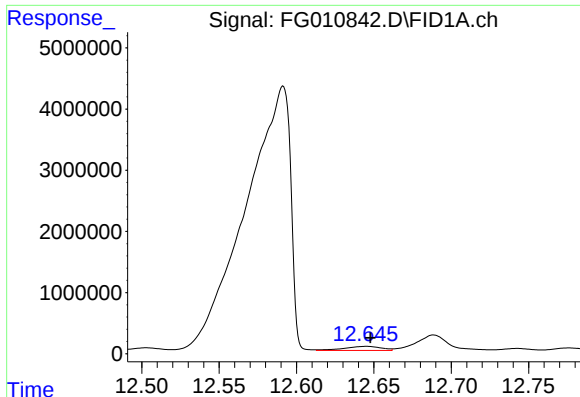

#7 N-EICOSANE


R.T.: 12.645 min
Delta R.T.: -0.003 min
Response: 1086491
Conc: 7.68 ug/ml

Instrument :
FID_G
ClientSampleId :

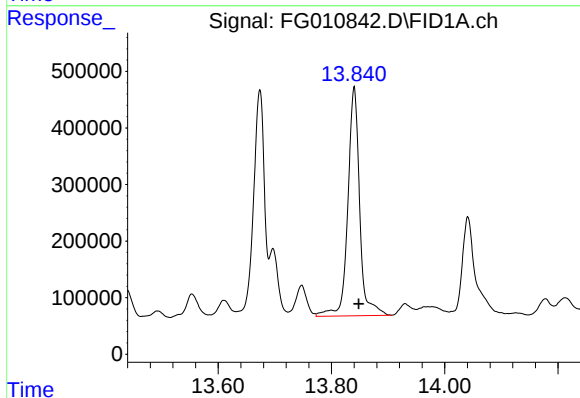


#8 N-DOCOSANE

R.T.: 13.840 min
Delta R.T.: -0.008 min
Response: 5866770
Conc: 42.38 ug/ml

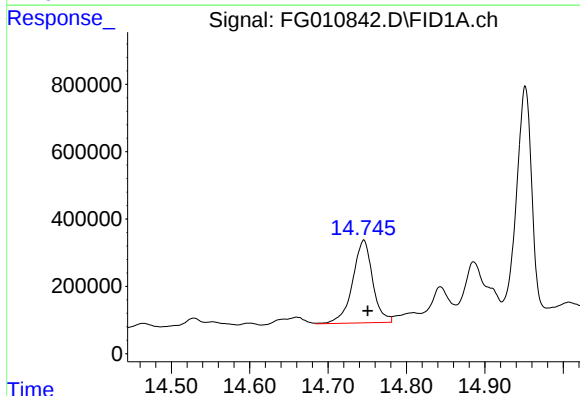


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.746 min
Delta R.T.: -0.005 min
Response: 4364918
Conc: 35.98 ug/ml

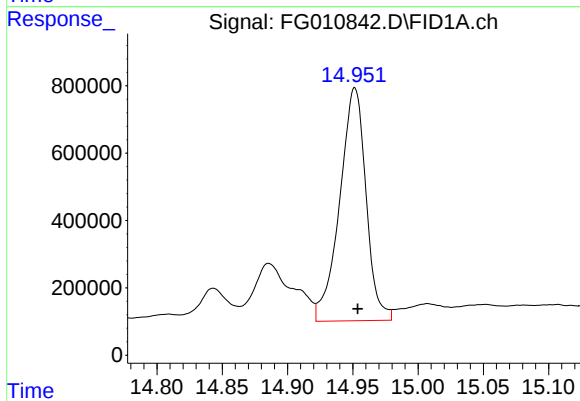

#10 N-TETRACOSANE


R.T.: 14.952 min
Delta R.T.: -0.002 min
Response: 9724715
Conc: 70.59 ug/ml

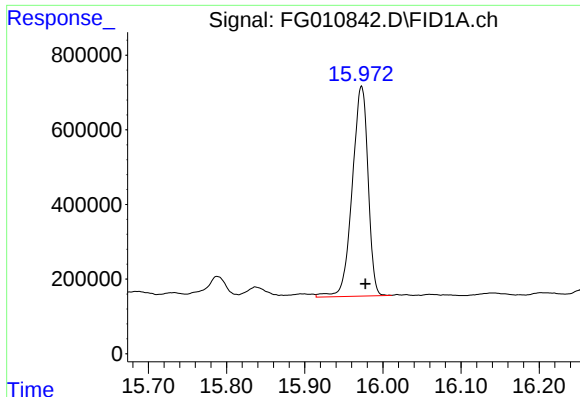

#11 N-HEXACOSANE


R.T.: 15.973 min
Delta R.T.: -0.005 min
Response: 7903434
Conc: 58.58 ug/ml

Instrument :
FID_G
ClientSampleId :

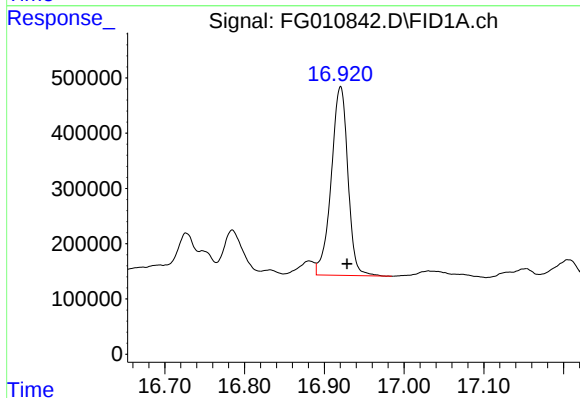


#12 N-OCTACOSANE

R.T.: 16.920 min
Delta R.T.: -0.008 min
Response: 4956162
Conc: 37.79 ug/ml

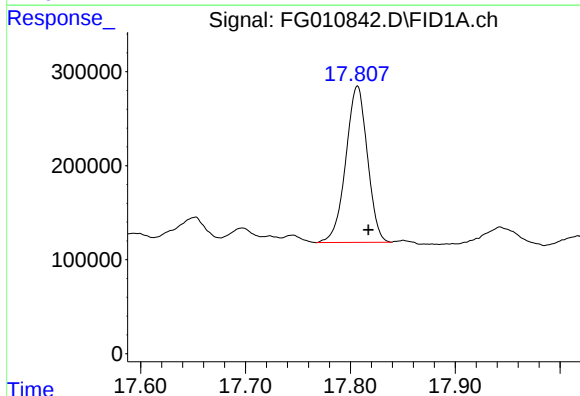


#13 N-TRIACONTANE

R.T.: 17.807 min
Delta R.T.: -0.010 min
Response: 2379629
Conc: 18.49 ug/ml

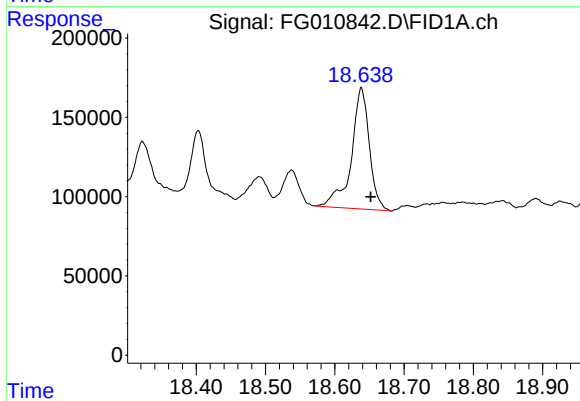

#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: -0.014 min
Response: 1383244
Conc: 10.89 ug/ml

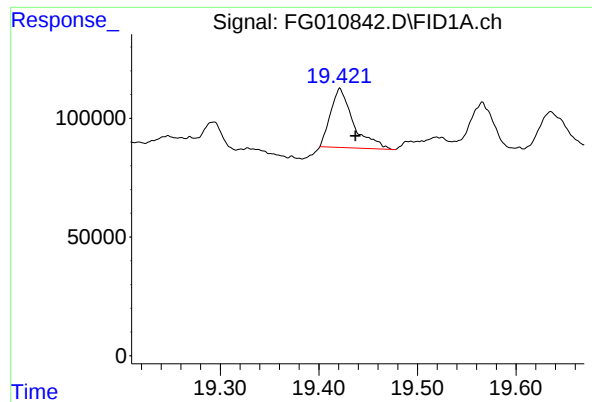

#15 N-TETRATRIACONTANE

R.T.: 19.421 min
Delta R.T.: -0.016 min
Response: 399488
Conc: 3.18 ug/ml

Instrument :

FID_G

ClientSampleId :