

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101122\
 Data File : FG010847.D
 Signal(s) : FID1A.ch
 Acq On : 11 Oct 2022 21:55
 Operator : YP\AJ
 Sample : N5067-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 12 07:51:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
 Quant Title :
 QLast Update : Thu Sep 29 02:21:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	1721541	14.190 ug/ml
Target Compounds			
7) N-EICOSANE	12.662	4467034	31.589 ug/ml
8) N-DOCOSANE	13.863	322989	2.333 ug/ml
10) N-TETRACOSANE	14.997	585558	4.250 ug/ml
12) N-OCTACOSANE	16.875f	471138	3.593 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101122\
Data File : FG010847.D
Signal(s) : FID1A.ch
Acq On : 11 Oct 2022 21:55
Operator : YP\AJ
Sample : N5067-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 12 07:51:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

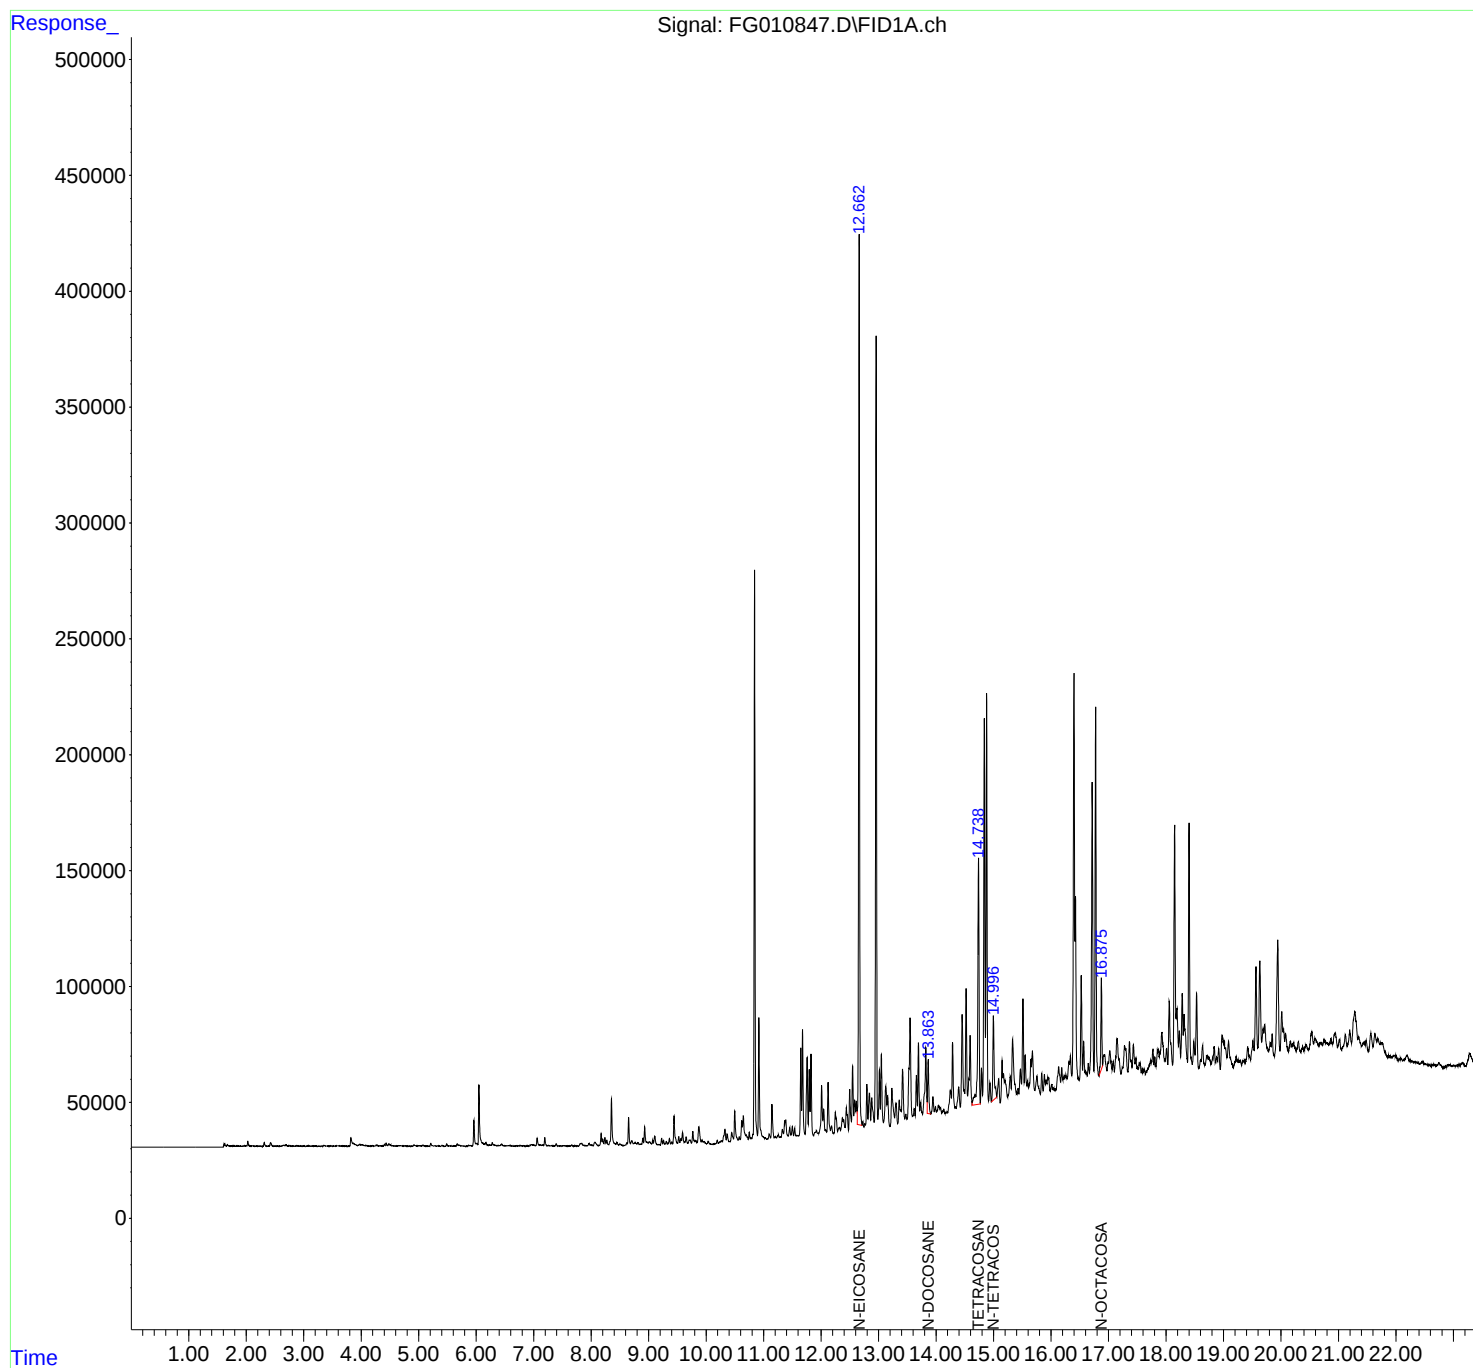


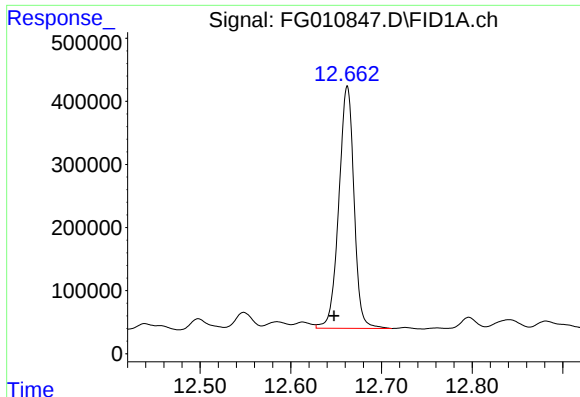

#7 N-EICOSANE


R.T.: 12.662 min
Delta R.T.: 0.014 min
Response: 4467034
Conc: 31.59 ug/ml

Instrument :
FID_G
ClientSampleId :

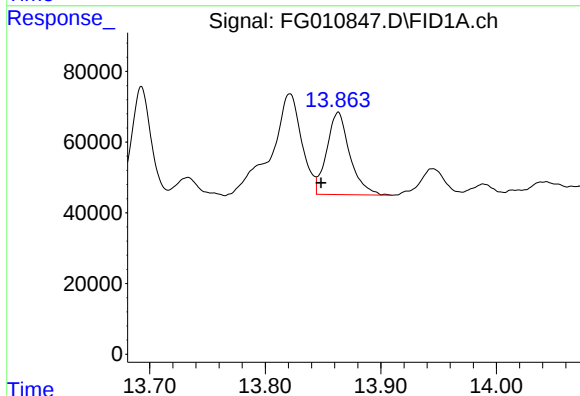


#8 N-DOCOSANE

R.T.: 13.863 min
Delta R.T.: 0.015 min
Response: 322989
Conc: 2.33 ug/ml

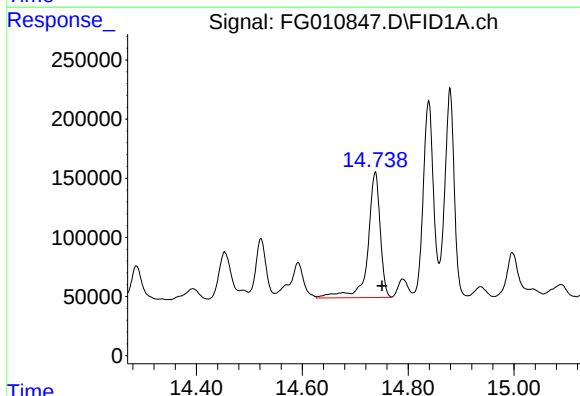


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: -0.013 min
Response: 1721541
Conc: 14.19 ug/ml

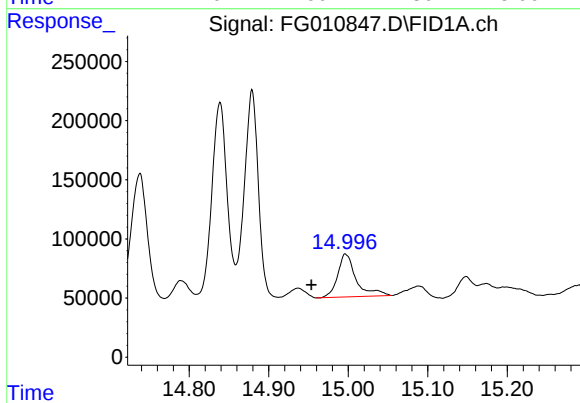

#10 N-TETRACOSANE

R.T.: 14.997 min
Delta R.T.: 0.043 min
Response: 585558
Conc: 4.25 ug/ml

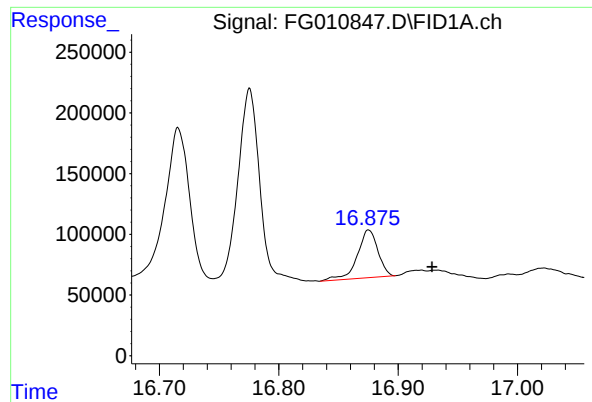

#12 N-OCTACOSANE

R.T.: 16.875 min
Delta R.T.: -0.053 min
Response: 471138
Conc: 3.59 ug/ml

Instrument :
FID_G
ClientSampleId :