

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101124\
Data File : FG014407.D
Signal(s) : FID1A.ch
Acq On : 11 Oct 2024 12:00
Operator : YP\AJ
Sample : PB164026BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB164026BL

Integration File: autoint1.e
Quant Time: Oct 14 03:00:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 05:57:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.914	2260709	18.257 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101124\
Data File : FG014407.D
Signal(s) : FID1A.ch
Acq On : 11 Oct 2024 12:00
Operator : YP\AJ
Sample : PB164026BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB164026BL

Integration File: autoint1.e
Quant Time: Oct 14 03:00:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 05:57:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

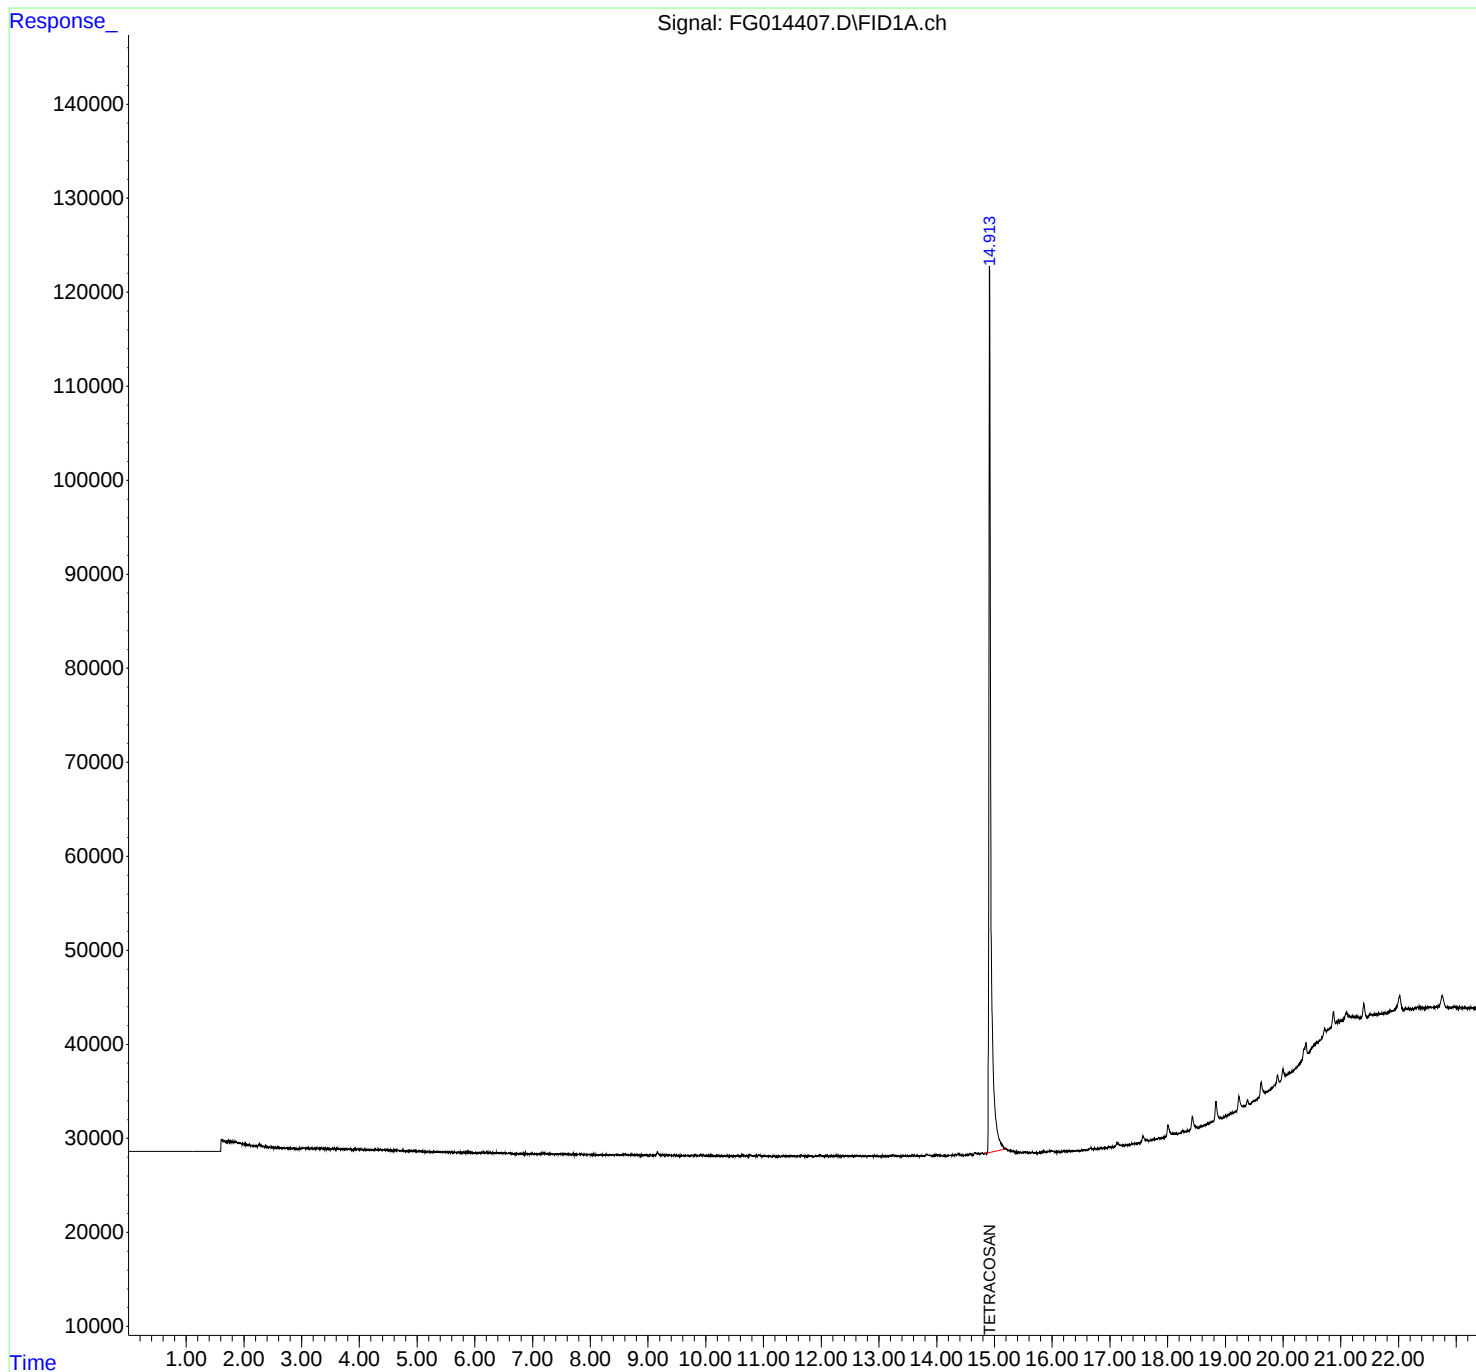

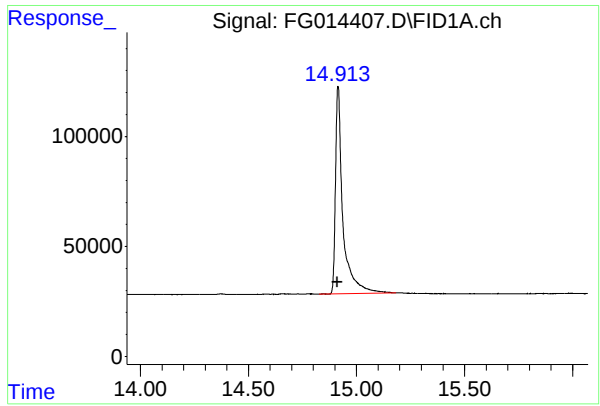

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.914 min
Delta R.T.: 0.003 min
Response: 2260709
Conc: 18.26 ug/ml

Instrument :
FID_G
ClientSampleId :
PB164026BL