

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101221\
Data File : FG008850.D
Signal(s) : FID1A.ch
Acq On : 12 Oct 2021 12:59
Operator : AJ\MA
Sample : M4146-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
20-SB-3-20211007-10.5-11.0

Integration File: autoint1.e
Quant Time: Oct 13 03:52:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	2248135	19.477 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101221\
Data File : FG008850.D
Signal(s) : FID1A.ch
Acq On : 12 Oct 2021 12:59
Operator : AJ\MA
Sample : M4146-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
20-SB-3-20211007-10.5-11.0

Integration File: autoint1.e
Quant Time: Oct 13 03:52:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

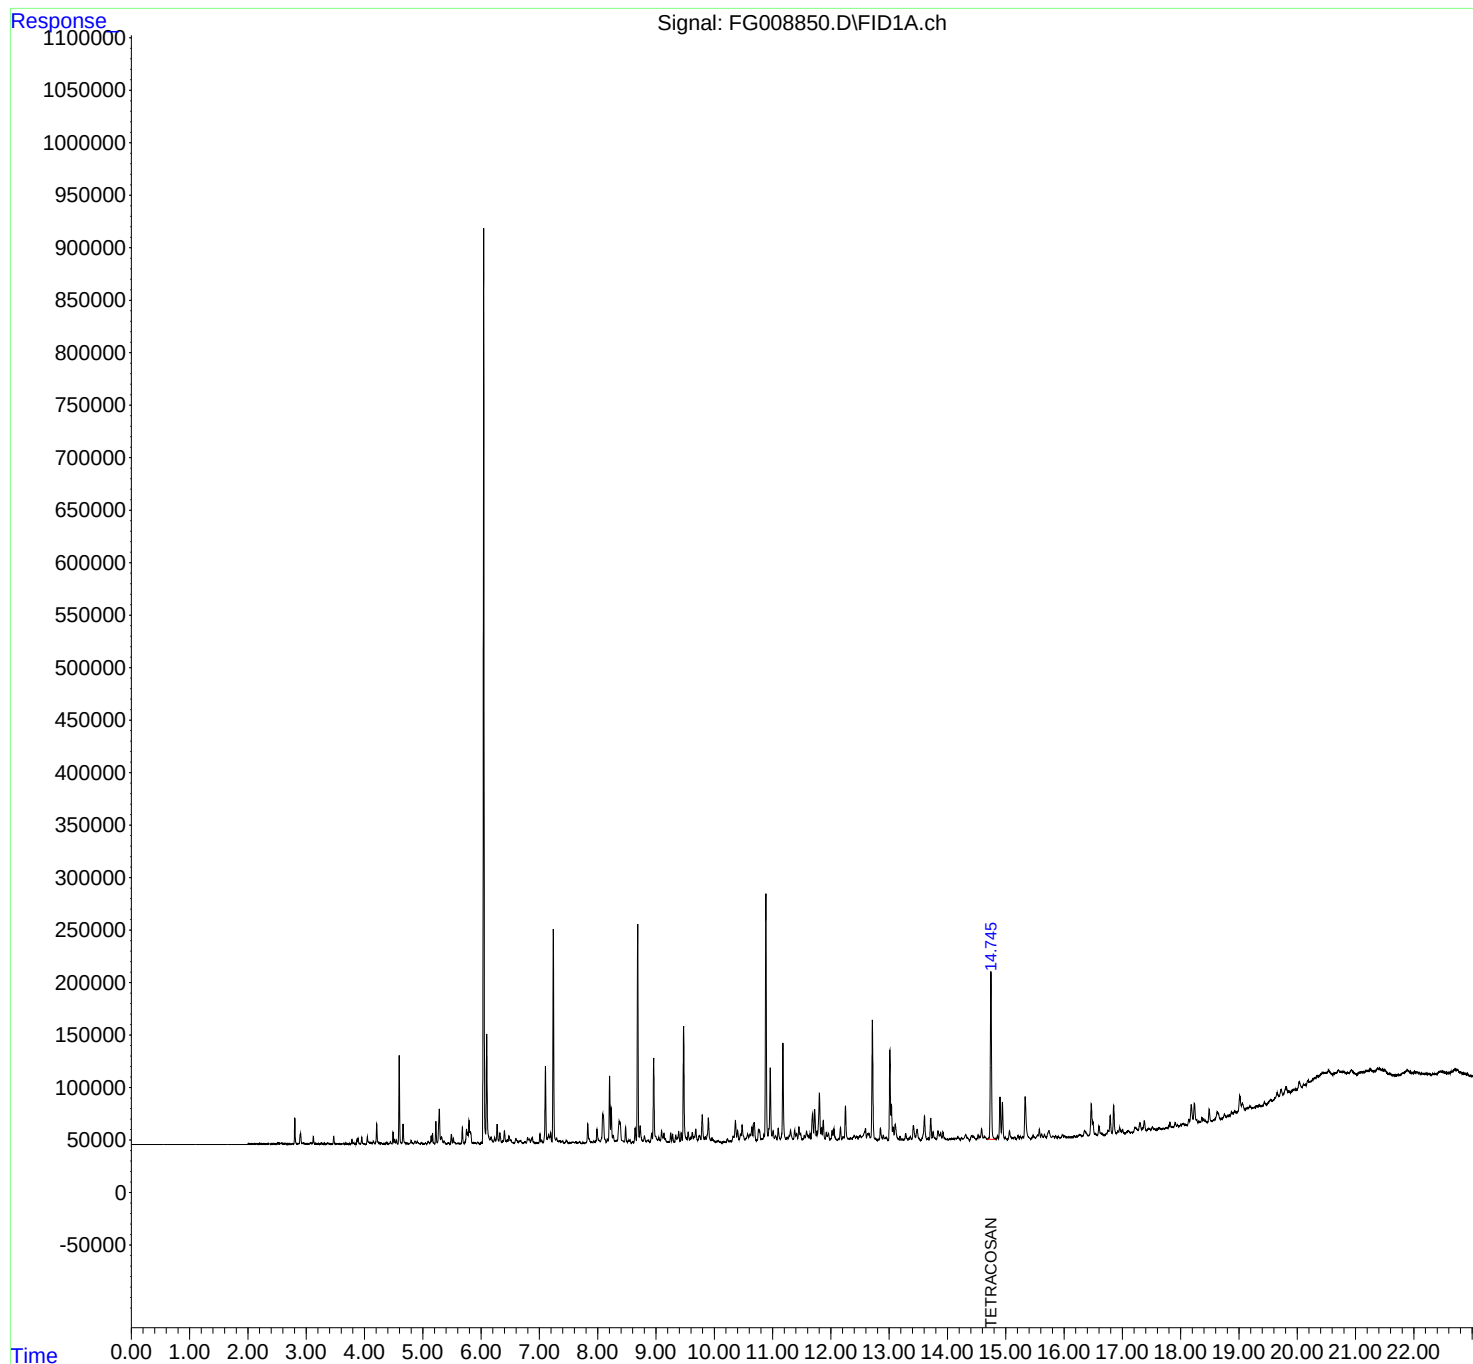

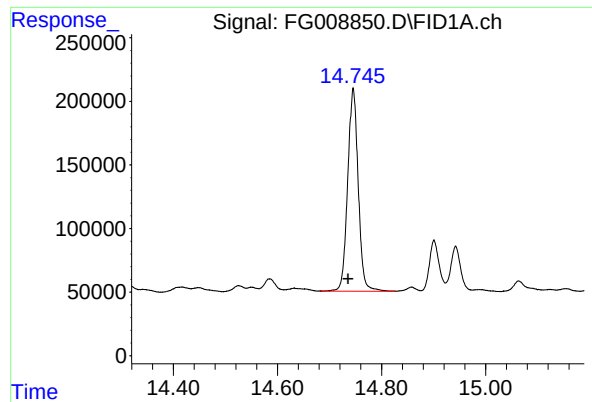

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.746 min
Delta R.T.: 0.010 min
Response: 2248135
Conc: 19.48 ug/ml

Instrument :
FID_G
ClientSampleId :
20-SB-3-20211007-10.5-11.0