

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101222\
 Data File : FG010886.D
 Signal(s) : FID1A.ch
 Acq On : 12 Oct 2022 20:38
 Operator : YP\AJ
 Sample : N5066-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 13 05:58:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
 Quant Title :
 QLast Update : Thu Sep 29 02:21:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	1516044	12.496 ug/ml
Target Compounds			
4) N-TETRADECANE	8.353f	299916	2.237 ug/ml
7) N-EICOSANE	12.664	3892676	27.528 ug/ml
10) N-TETRACOSANE	15.000	269217	1.954 ug/ml
12) N-OCTACOSANE	16.915	353495	2.696 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101222\
Data File : FG010886.D
Signal(s) : FID1A.ch
Acq On : 12 Oct 2022 20:38
Operator : YP\AJ
Sample : N5066-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 13 05:58:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

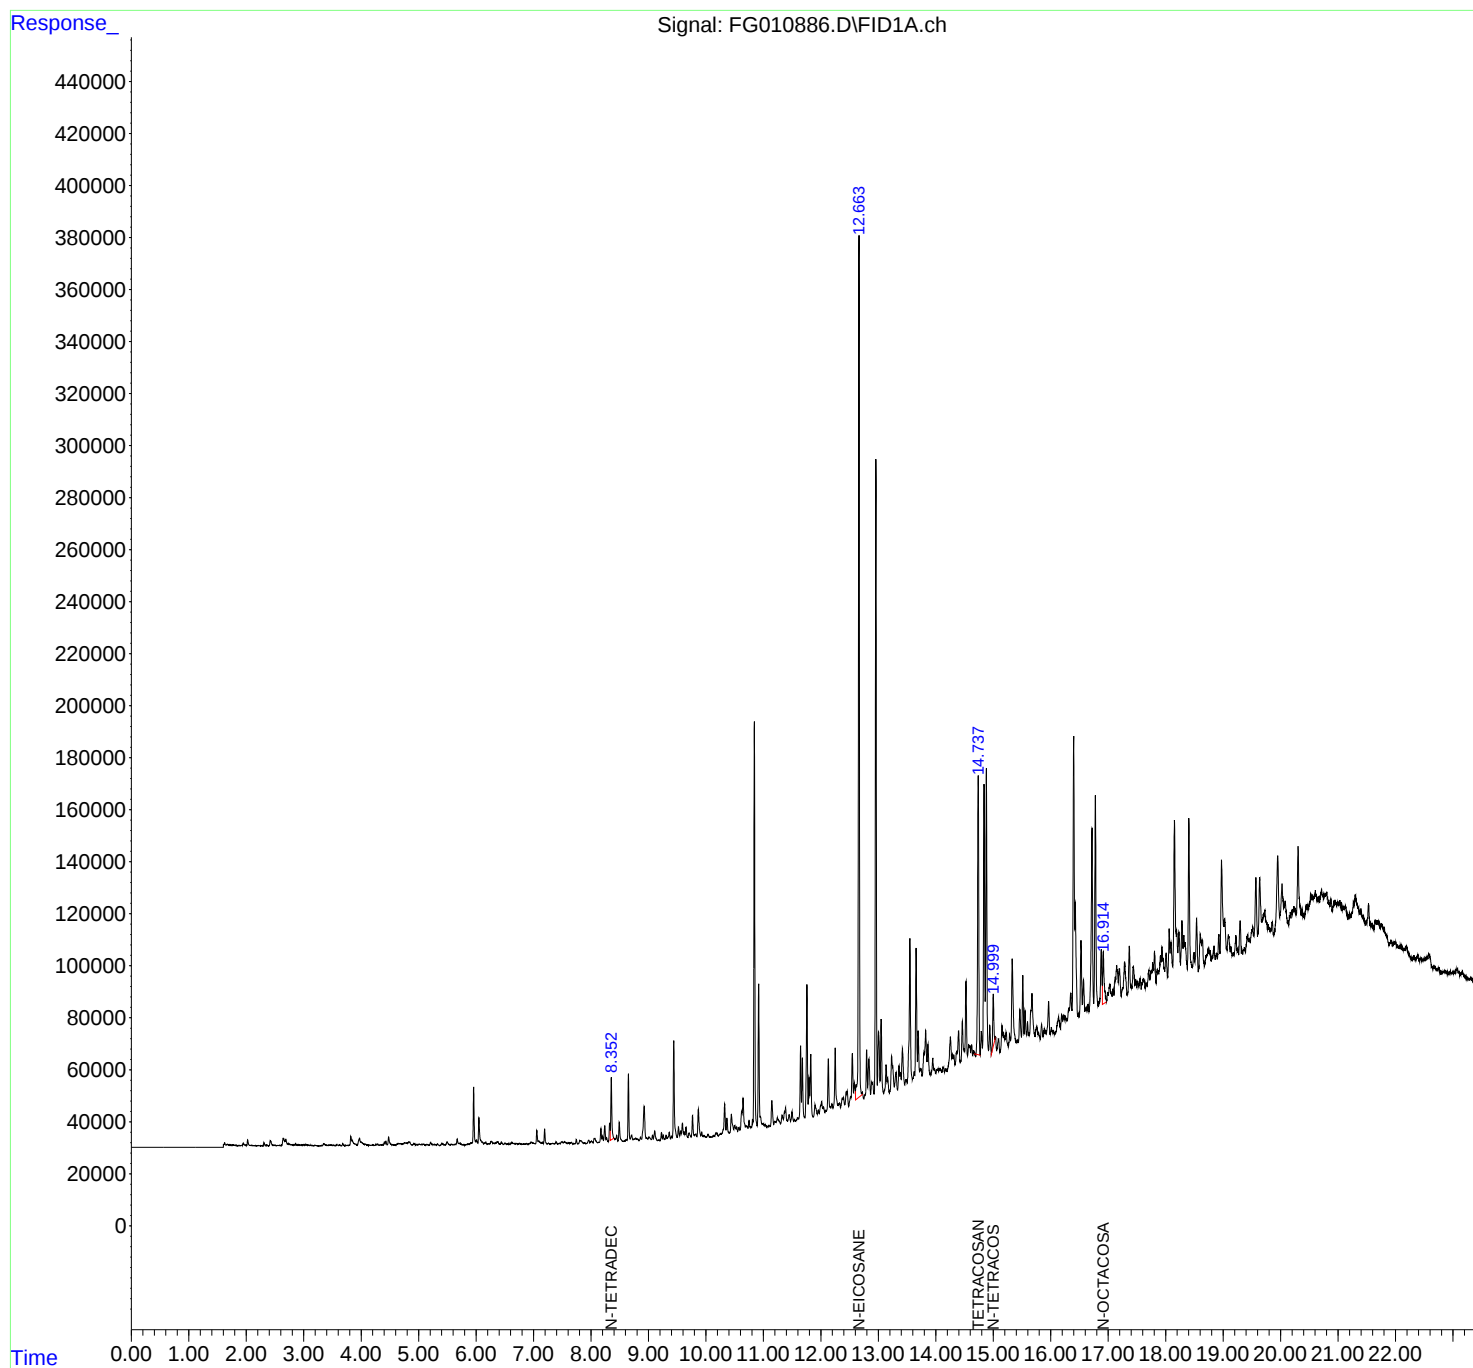


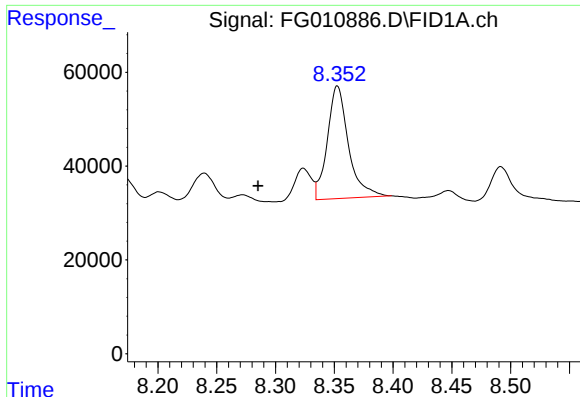

#4 N-TETRADECANE


R.T.: 8.353 min
Delta R.T.: 0.067 min
Response: 299916
Conc: 2.24 ug/ml

Instrument :
FID_G
ClientSampleId :

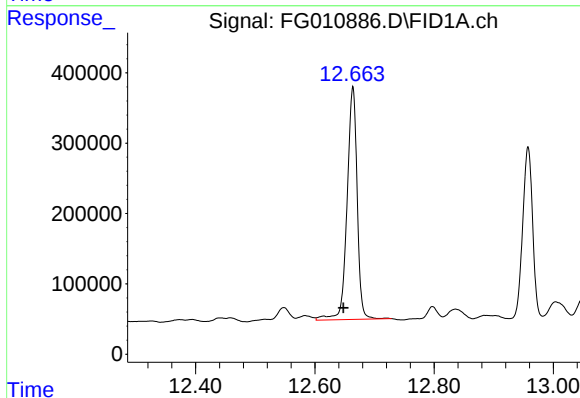


#7 N-EICOSANE

R.T.: 12.664 min
Delta R.T.: 0.016 min
Response: 3892676
Conc: 27.53 ug/ml

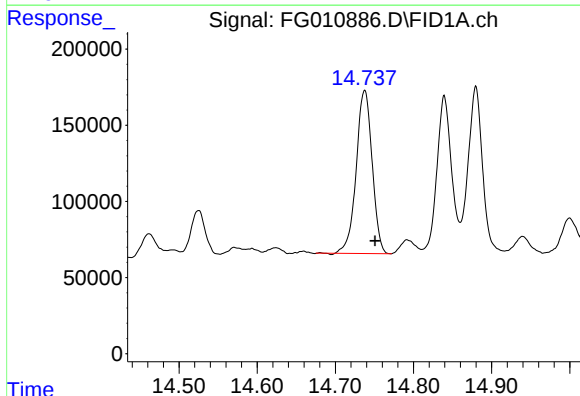


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: -0.013 min
Response: 1516044
Conc: 12.50 ug/ml

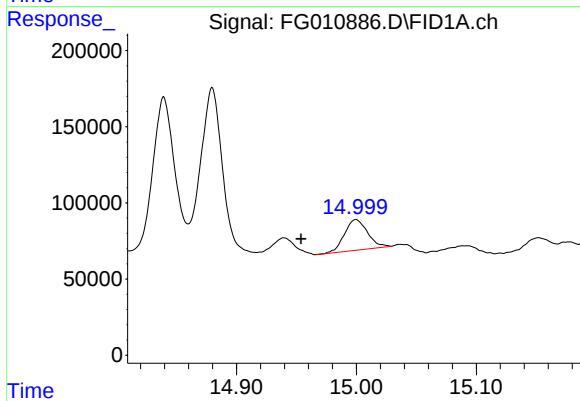

#10 N-TETRACOSANE

R.T.: 15.000 min
Delta R.T.: 0.046 min
Response: 269217
Conc: 1.95 ug/ml

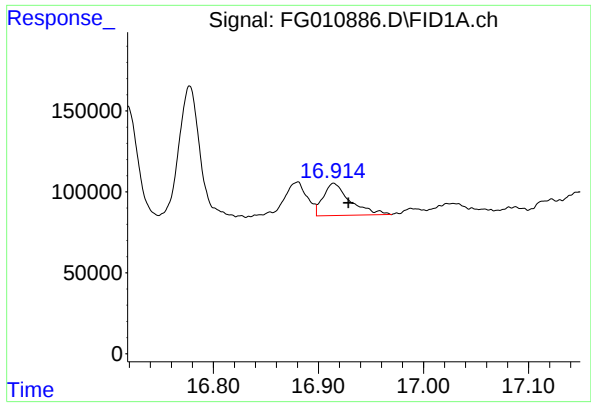

#12 N-OCTACOSANE

R.T.: 16.915 min
Delta R.T.: -0.014 min
Response: 353495
Conc: 2.70 ug/ml

Instrument :
FID_G
ClientSampleId :