

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101320\
 Data File : FG007180.D
 Signal(s) : FID1A.ch
 Acq On : 13 Oct 2020 19:47
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 14 00:53:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
 Quant Title :
 QLast Update : Mon Oct 05 13:04:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.752	4975646	40.863 ug/ml
Target Compounds			
2) N-DECANE	4.450	6229535	45.914 ug/ml
3) N-DODECANE	6.479	6207471	45.295 ug/ml
4) N-TETRADECANE	8.281	6085921	44.592 ug/ml
5) N-HEXADECANE	9.887	6127625	43.510 ug/ml
6) N-OCTADECANE	11.334	6076501	42.670 ug/ml
7) N-EICOSANE	12.647	5934772	41.954 ug/ml
8) N-DOCOSANE	13.850	5771388	41.346 ug/ml
10) N-TETRACOSANE	14.956	5703060	40.878 ug/ml
11) N-HEXACOSANE	15.979	5556107	40.557 ug/ml
12) N-OCTACOSANE	16.932	5465541	40.524 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101320\
Data File : FG007180.D
Signal(s) : FID1A.ch
Acq On : 13 Oct 2020 19:47
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 14 00:53:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
Quant Title :
QLast Update : Mon Oct 05 13:04:52 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

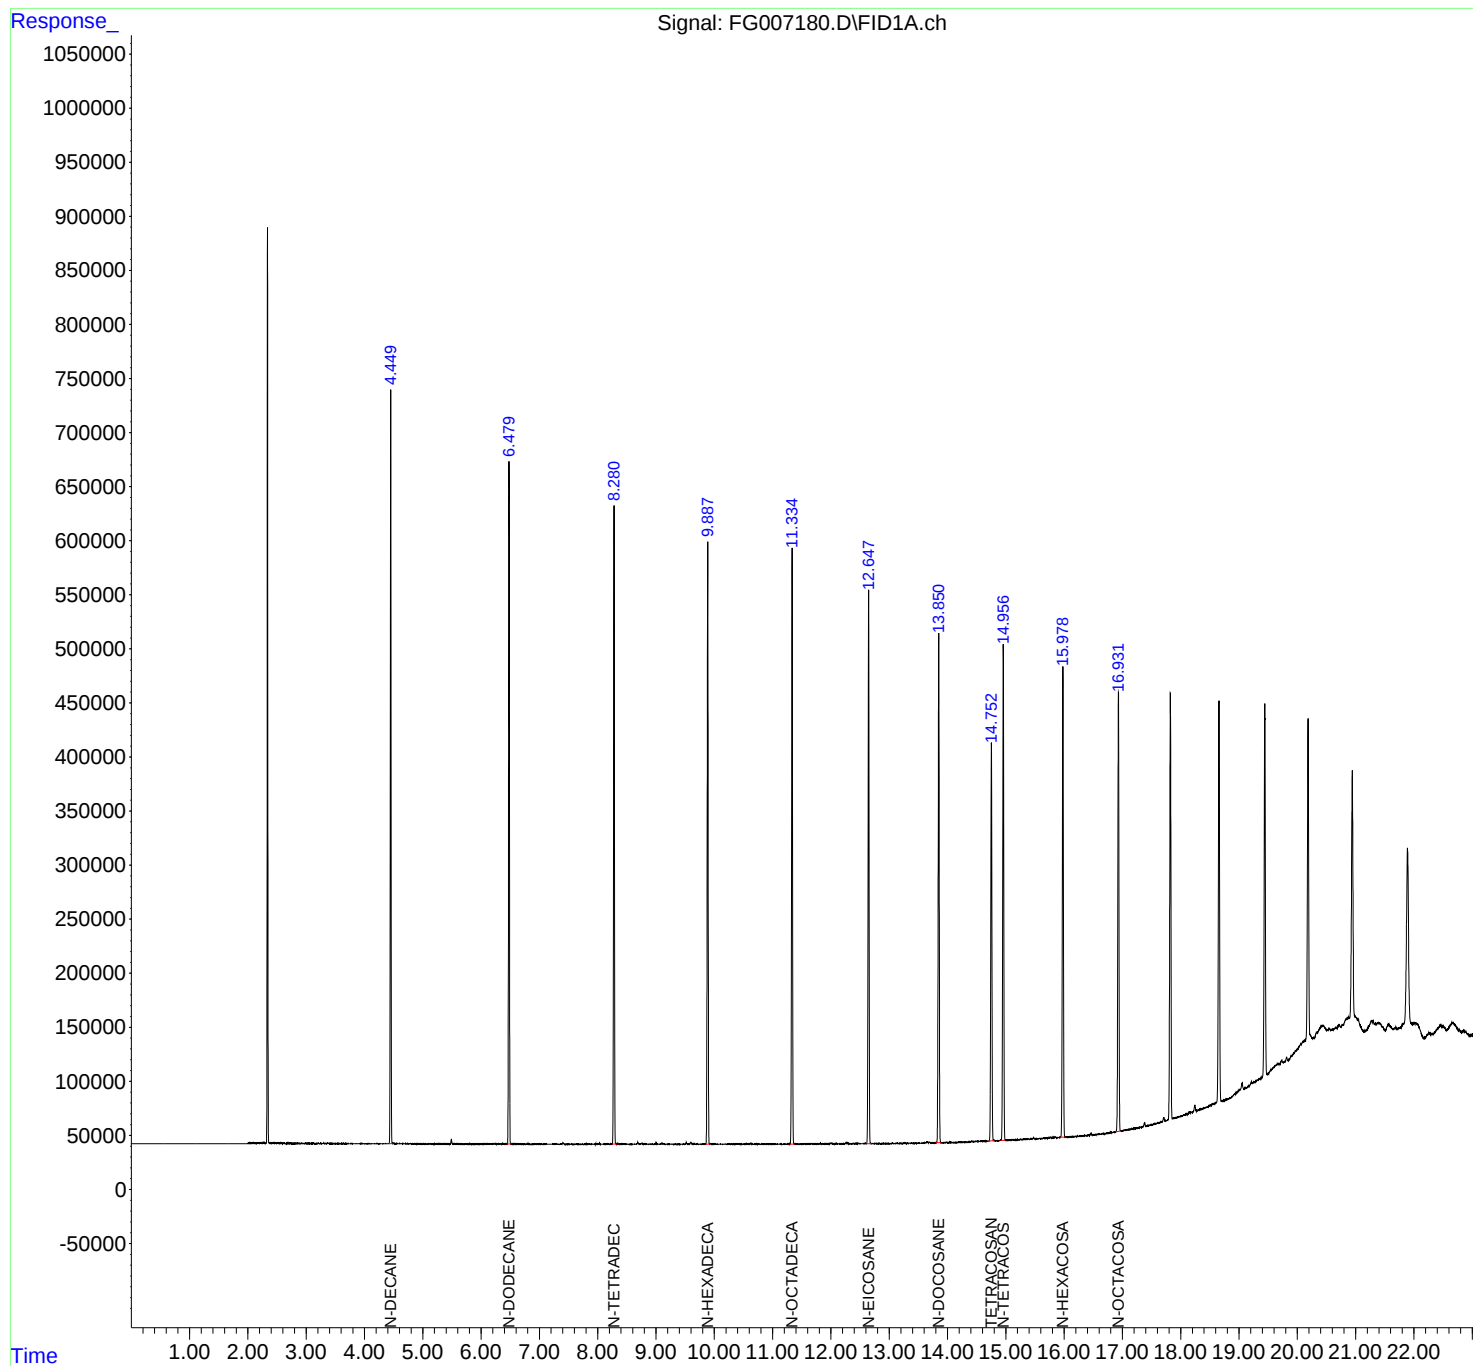

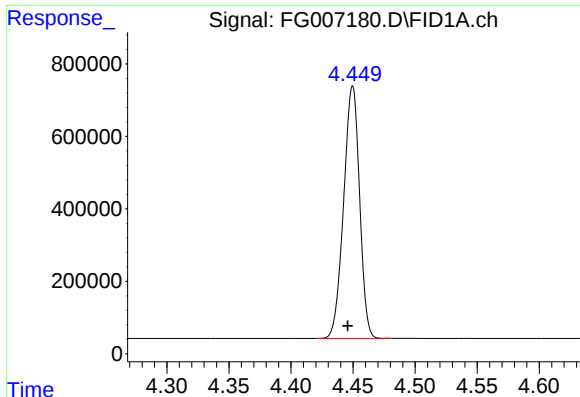


#2 N-DECANE

R.T.: 4.450 min
Delta R.T.: 0.004 min
Response: 6229535
Conc: 45.91 ug/ml

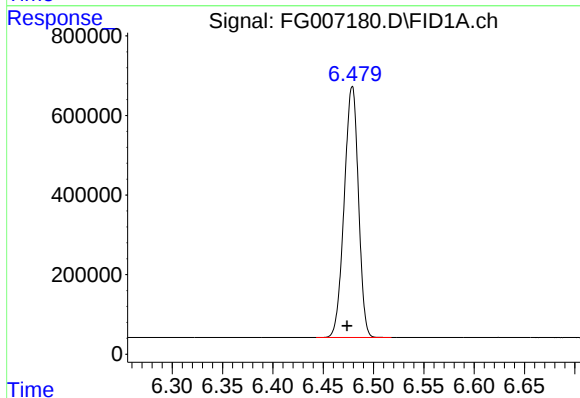


#3 N-DODECANE

R.T.: 6.479 min
Delta R.T.: 0.005 min
Response: 6207471
Conc: 45.29 ug/ml

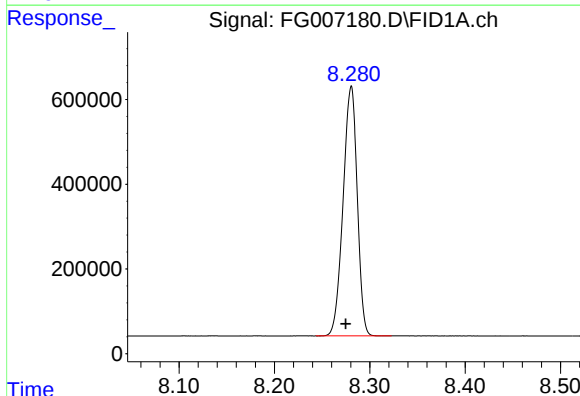


#4 N-TETRADECANE

R.T.: 8.281 min
Delta R.T.: 0.006 min
Response: 6085921
Conc: 44.59 ug/ml

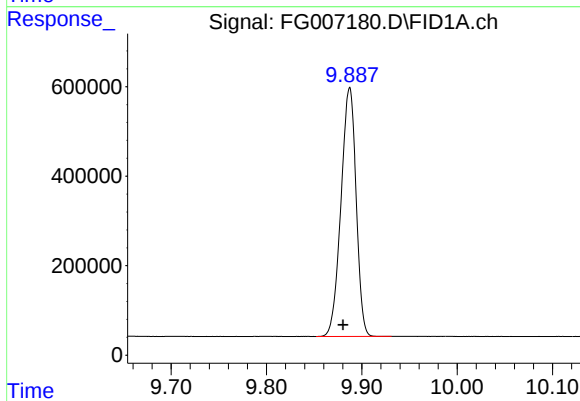


#5 N-HEXADECANE

R.T.: 9.887 min
Delta R.T.: 0.007 min
Response: 6127625
Conc: 43.51 ug/ml

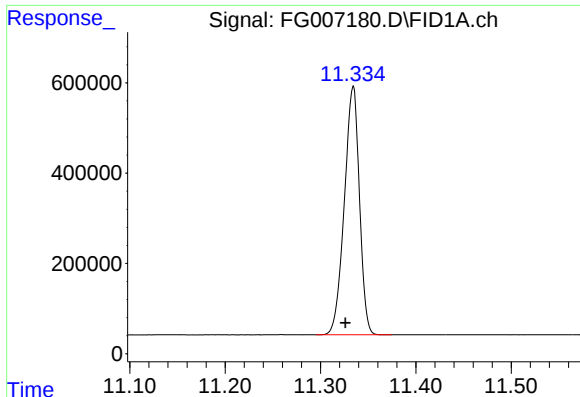


#6 N-OCTADECANE

R.T.: 11.334 min
Delta R.T.: 0.008 min
Response: 6076501
Conc: 42.67 ug/ml

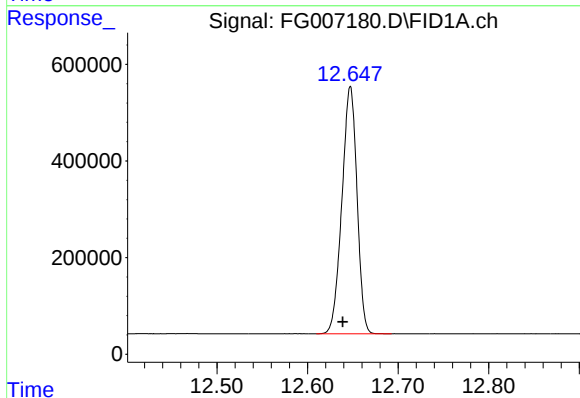


#7 N-EICOSANE

R.T.: 12.647 min
Delta R.T.: 0.008 min
Response: 5934772
Conc: 41.95 ug/ml

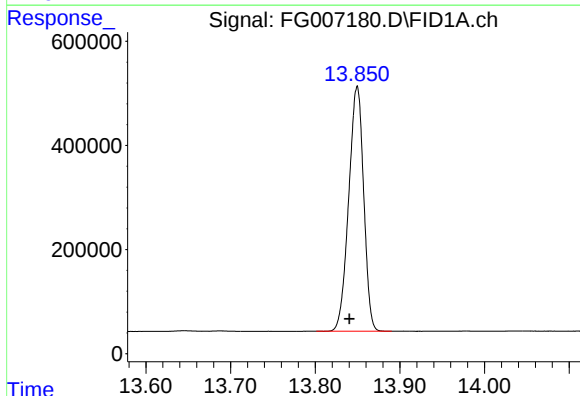


#8 N-DOCOSANE

R.T.: 13.850 min
Delta R.T.: 0.009 min
Response: 5771388
Conc: 41.35 ug/ml

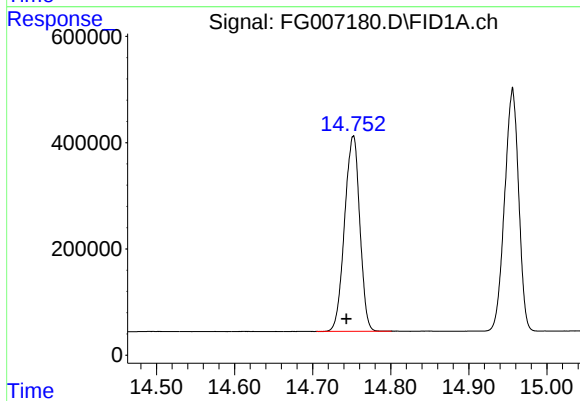


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.752 min
Delta R.T.: 0.009 min
Response: 4975646
Conc: 40.86 ug/ml

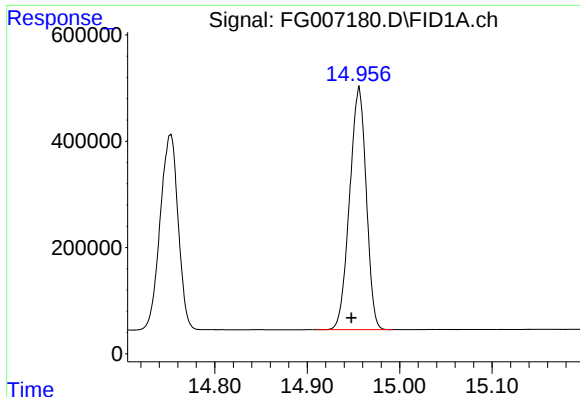


#10 N-TETRACOSANE

R.T.: 14.956 min
Delta R.T.: 0.008 min
Response: 5703060
Conc: 40.88 ug/ml

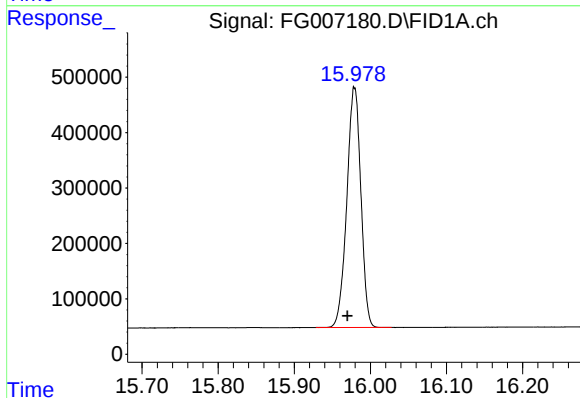

#11 N-HEXACOSANE

R.T.: 15.979 min
Delta R.T.: 0.009 min
Response: 5556107
Conc: 40.56 ug/ml

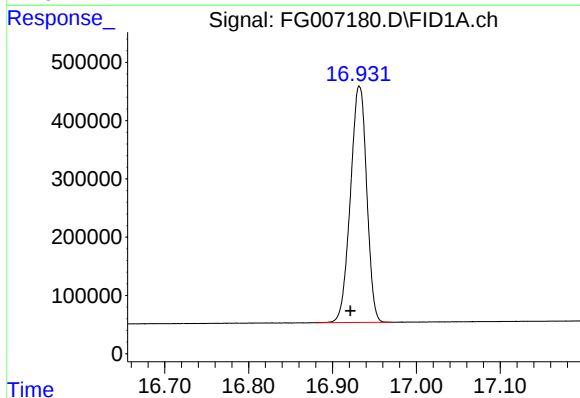

#12 N-OCTACOSANE

R.T.: 16.932 min
Delta R.T.: 0.011 min
Response: 5465541
Conc: 40.52 ug/ml