

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101322\
 Data File : FG010893.D
 Signal(s) : FID1A.ch
 Acq On : 13 Oct 2022 08:32
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2022
 Supervised By :Ankita Jodhani 10/13/2022

Integration File: autoint1.e
 Quant Time: Oct 13 10:44:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
 Quant Title :
 QLast Update : Thu Sep 29 02:21:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	2516399	20.742 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101322\
Data File : FG010893.D
Signal(s) : FID1A.ch
Acq On : 13 Oct 2022 08:32
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2022
Supervised By :Ankita Jodhani 10/13/2022

Integration File: autoint1.e
Quant Time: Oct 13 10:44:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

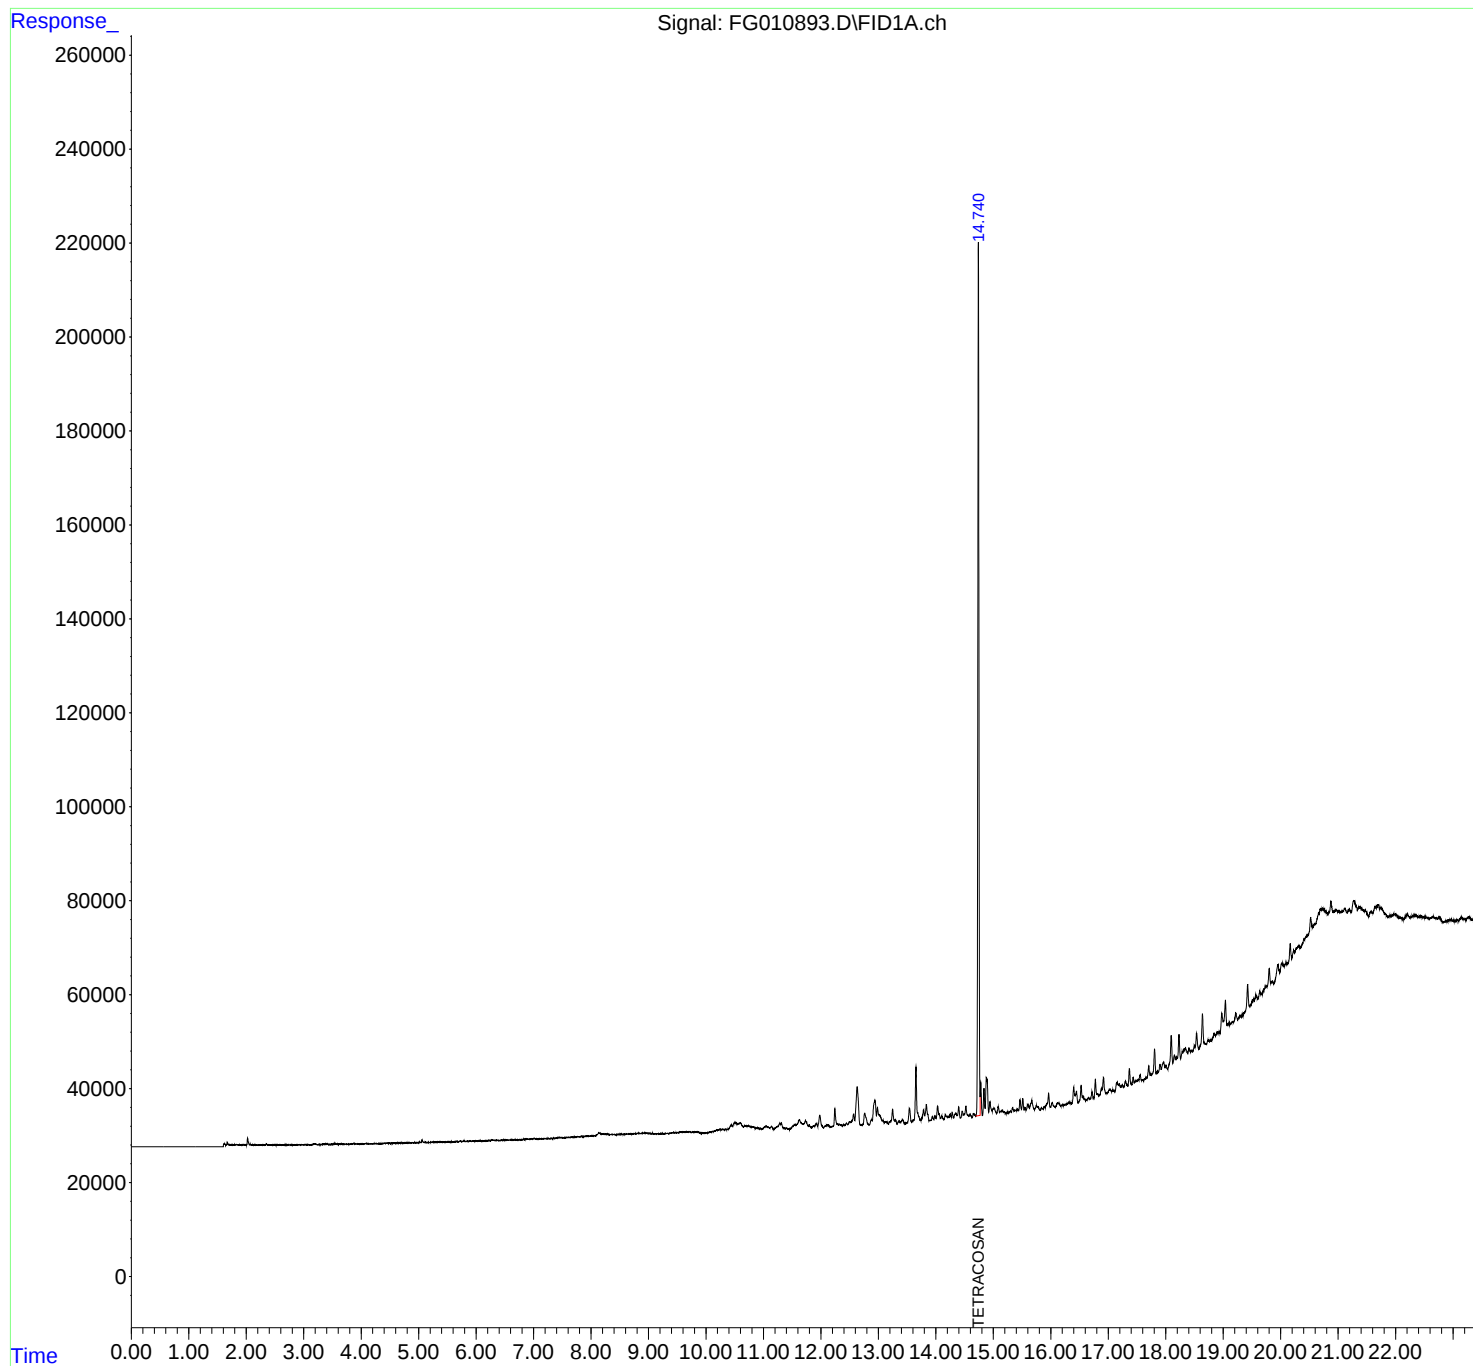

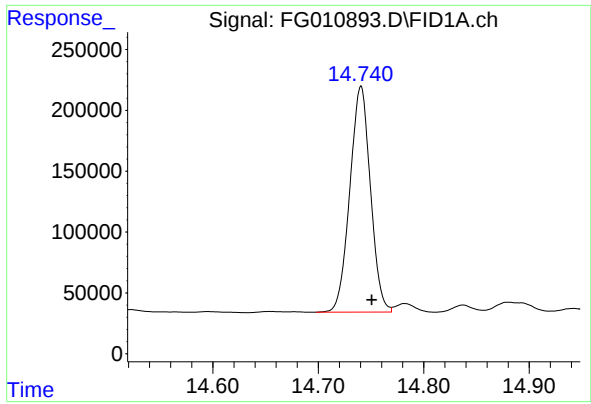

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: -0.010 min
Response: 2516399
Conc: 20.74 ug/ml

Instrument :

FID_G

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 10/13/2022

Supervised By :Ankita Jodhani 10/13/2022