

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101518\
 Data File : FG002608.D
 Signal(s) : FID1A.ch
 Acq On : 15 Oct 2018 15:19
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 15 15:41:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:36:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.767	5935338	51.710 ug/ml
Target Compounds			
2) N-DECANE	4.464	7249335	55.639 ug/ml
3) N-DODECANE	6.496	7283833	55.193 ug/ml
4) N-TETRADECANE	8.297	7277329	54.580 ug/ml
5) N-HEXADECANE	9.903	7241546	53.982 ug/ml
6) N-OCTADECANE	11.349	7187944	53.373 ug/ml
7) N-EICOSANE	12.663	7048330	52.840 ug/ml
8) N-DOCOSANE	13.867	6930981	52.526 ug/ml
10) N-TETRACOSANE	14.972	6833909	52.568 ug/ml
11) N-HEXACOSANE	15.997	6751868	52.562 ug/ml
12) N-OCTACOSANE	16.949	6794362	53.590 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101518\
Data File : FG002608.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2018 15:19
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 15 15:41:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

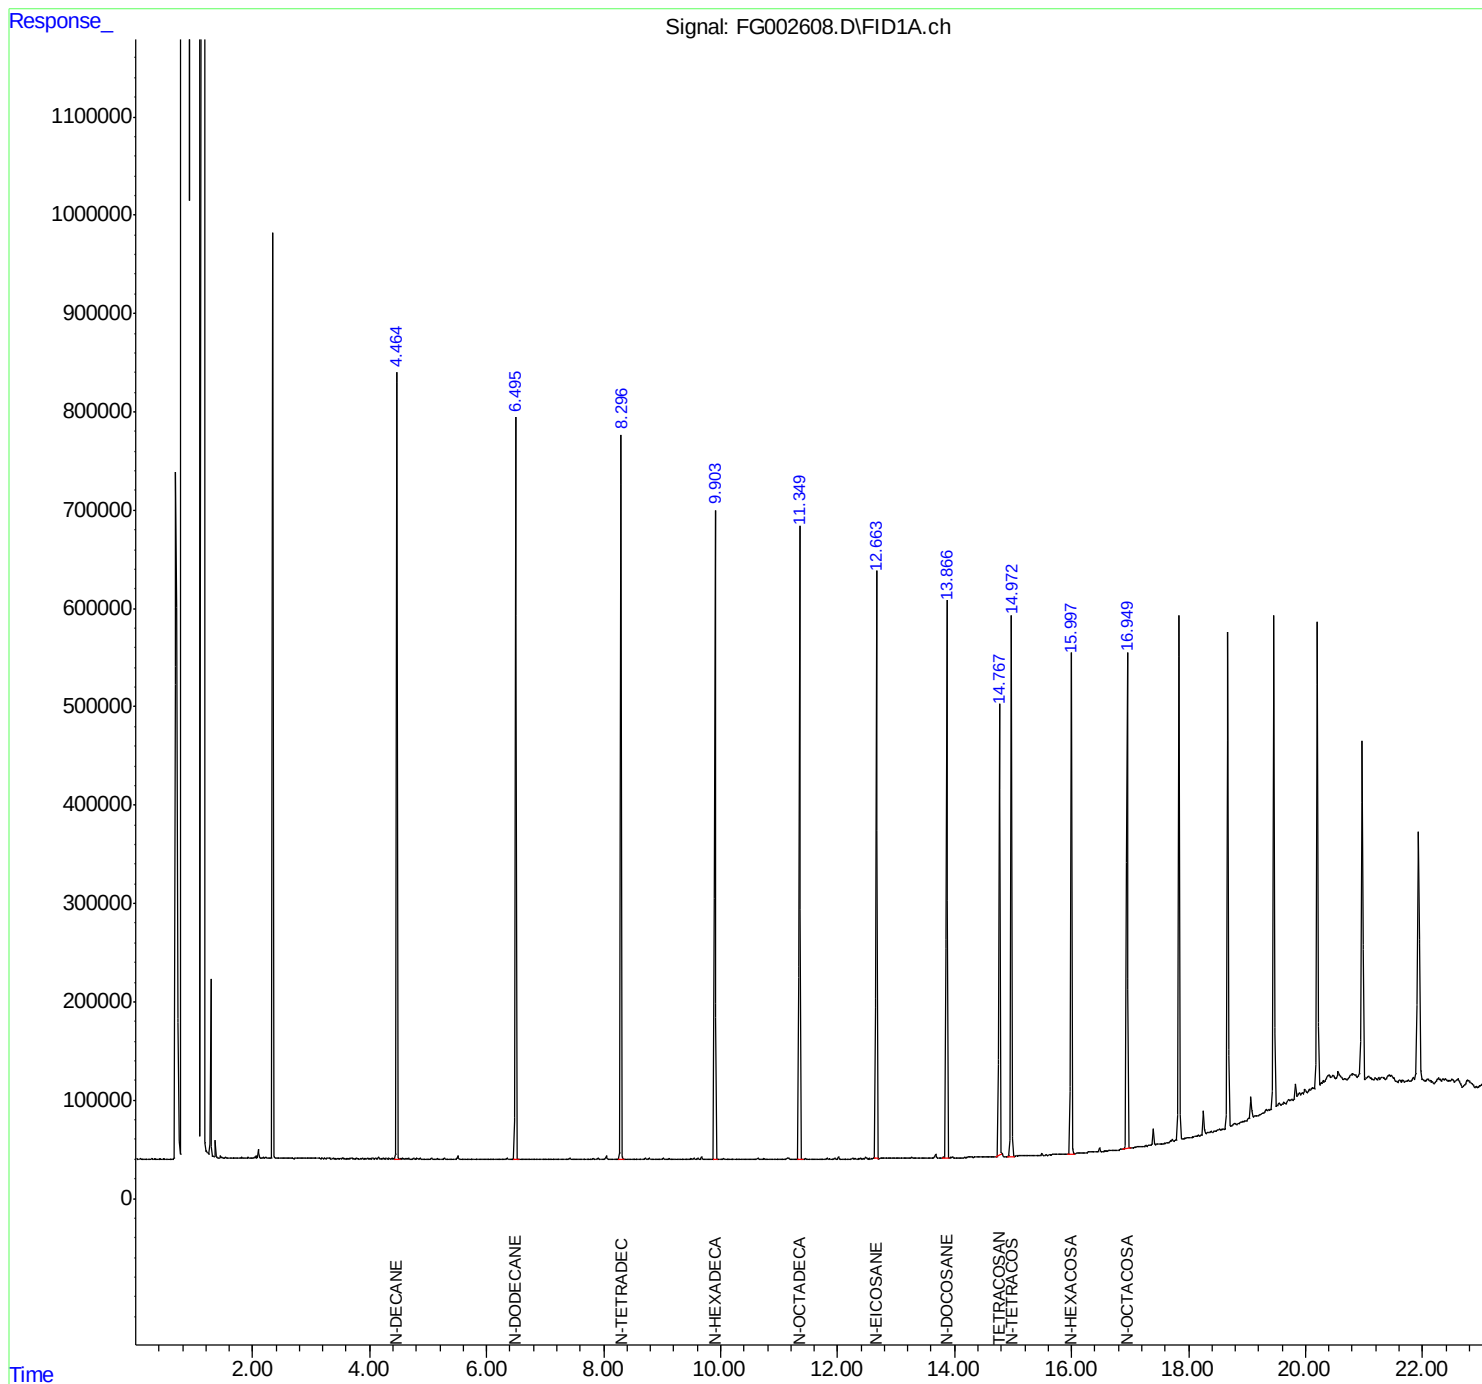

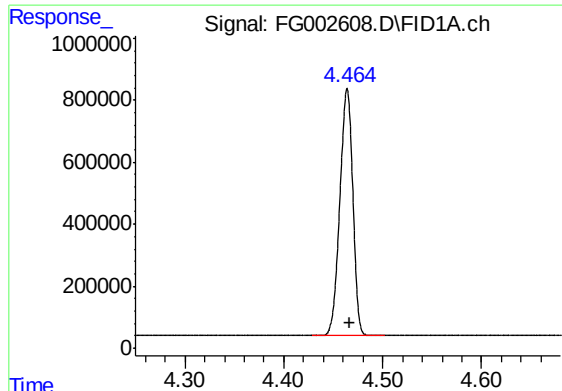


#2 N-DECANE

R.T.: 4.464 min
Delta R.T.: -0.003 min
Response: 7249335
Conc: 55.64 ug/ml

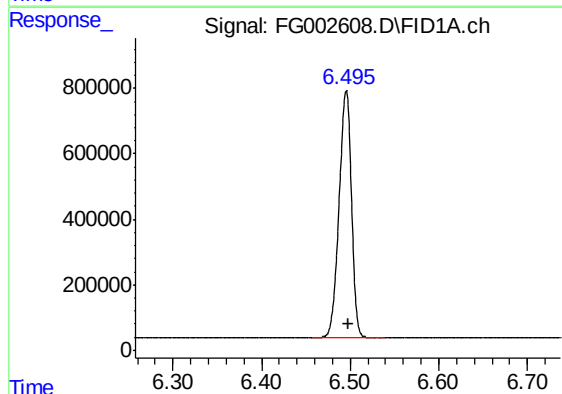


#3 N-DODECANE

R.T.: 6.496 min
Delta R.T.: -0.002 min
Response: 7283833
Conc: 55.19 ug/ml

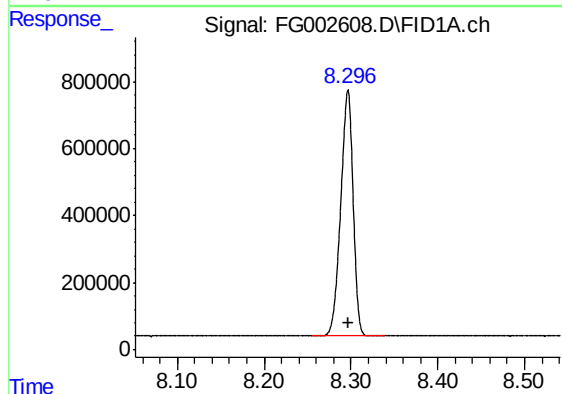


#4 N-TETRADECANE

R.T.: 8.297 min
Delta R.T.: -0.001 min
Response: 7277329
Conc: 54.58 ug/ml

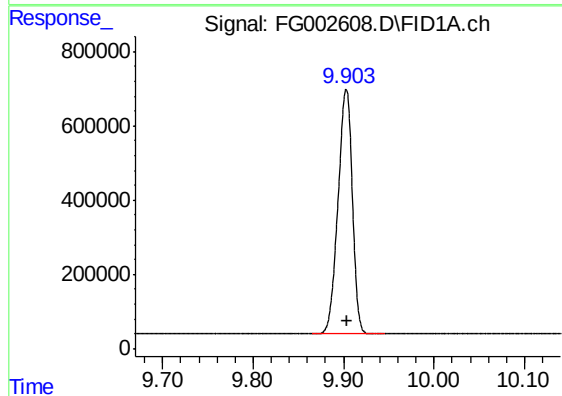


#5 N-HEXADECANE

R.T.: 9.903 min
Delta R.T.: 0.000 min
Response: 7241546
Conc: 53.98 ug/ml

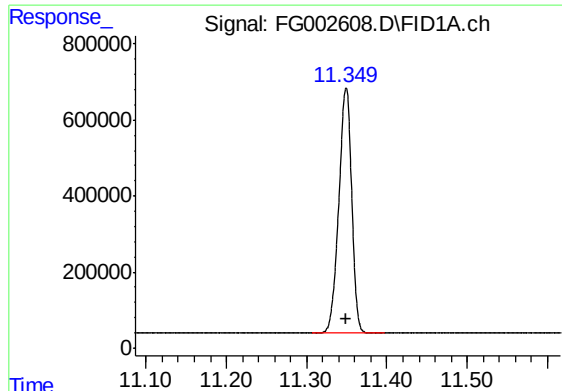


#6 N-OCTADECANE

R.T.: 11.349 min
Delta R.T.: 0.000 min
Response: 7187944
Conc: 53.37 ug/ml

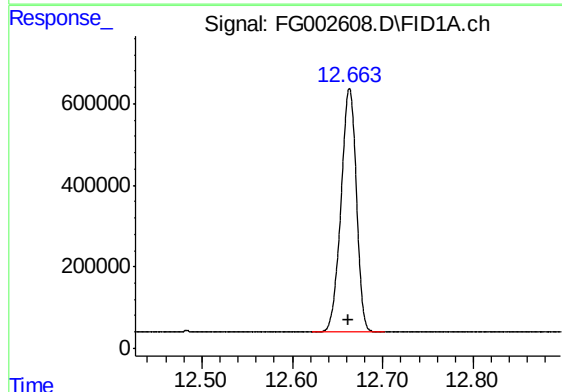


#7 N-EICOSANE

R.T.: 12.663 min
Delta R.T.: 0.000 min
Response: 7048330
Conc: 52.84 ug/ml

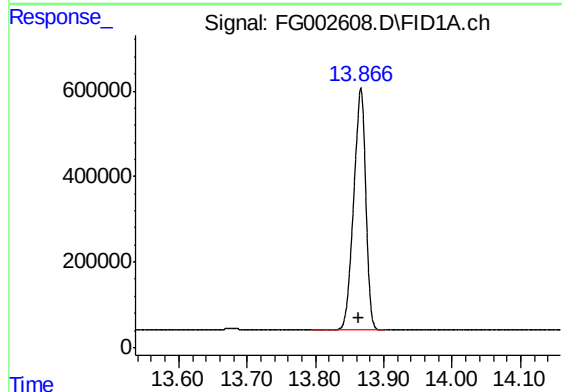


#8 N-DOCOSANE

R.T.: 13.867 min
Delta R.T.: 0.002 min
Response: 6930981
Conc: 52.53 ug/ml

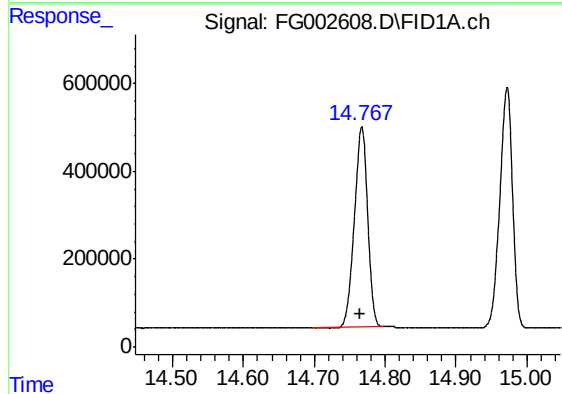


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.767 min
Delta R.T.: 0.002 min
Response: 5935338
Conc: 51.71 ug/ml

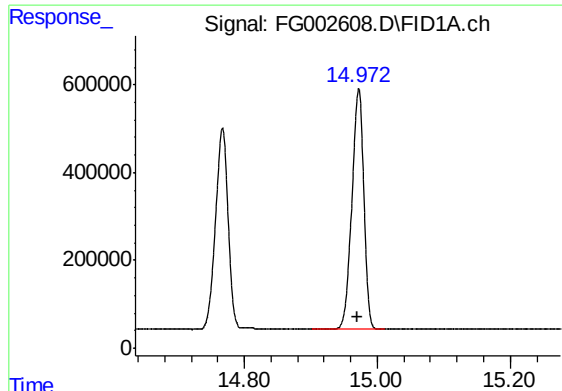


#10 N-TETRACOSANE

R.T.: 14.972 min
Delta R.T.: 0.002 min
Response: 6833909
Conc: 52.57 ug/ml

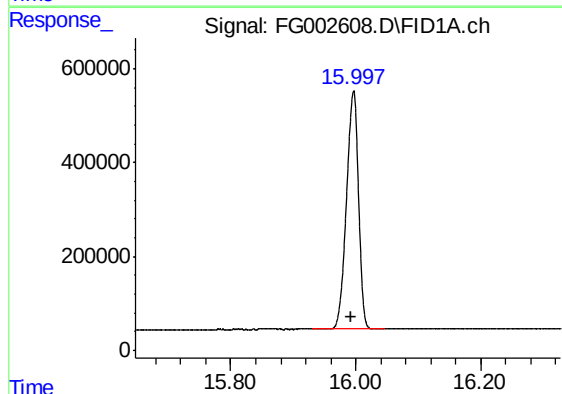

#11 N-HEXACOSANE

R.T.: 15.997 min
Delta R.T.: 0.003 min
Response: 6751868
Conc: 52.56 ug/ml

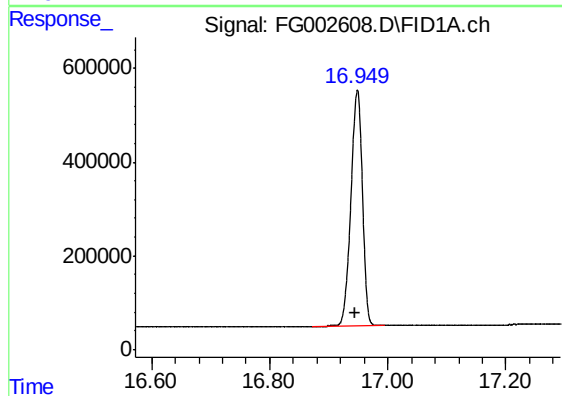

#12 N-OCTACOSANE

R.T.: 16.949 min
Delta R.T.: 0.004 min
Response: 6794362
Conc: 53.59 ug/ml