

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
 Data File : FG008882.D
 Signal(s) : FID1A.ch
 Acq On : 15 Oct 2021 09:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 16 00:49:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
 Quant Title :
 QLast Update : Fri Oct 08 03:31:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.739	2195139	19.018 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.814	53264	0.470 ug/ml
14) N-DOTRIACONTANE	18.647	73788	0.696 ug/ml
15) N-TETRATRIACONTANE	19.433	49147	0.493 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
Data File : FG008882.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2021 09:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:49:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

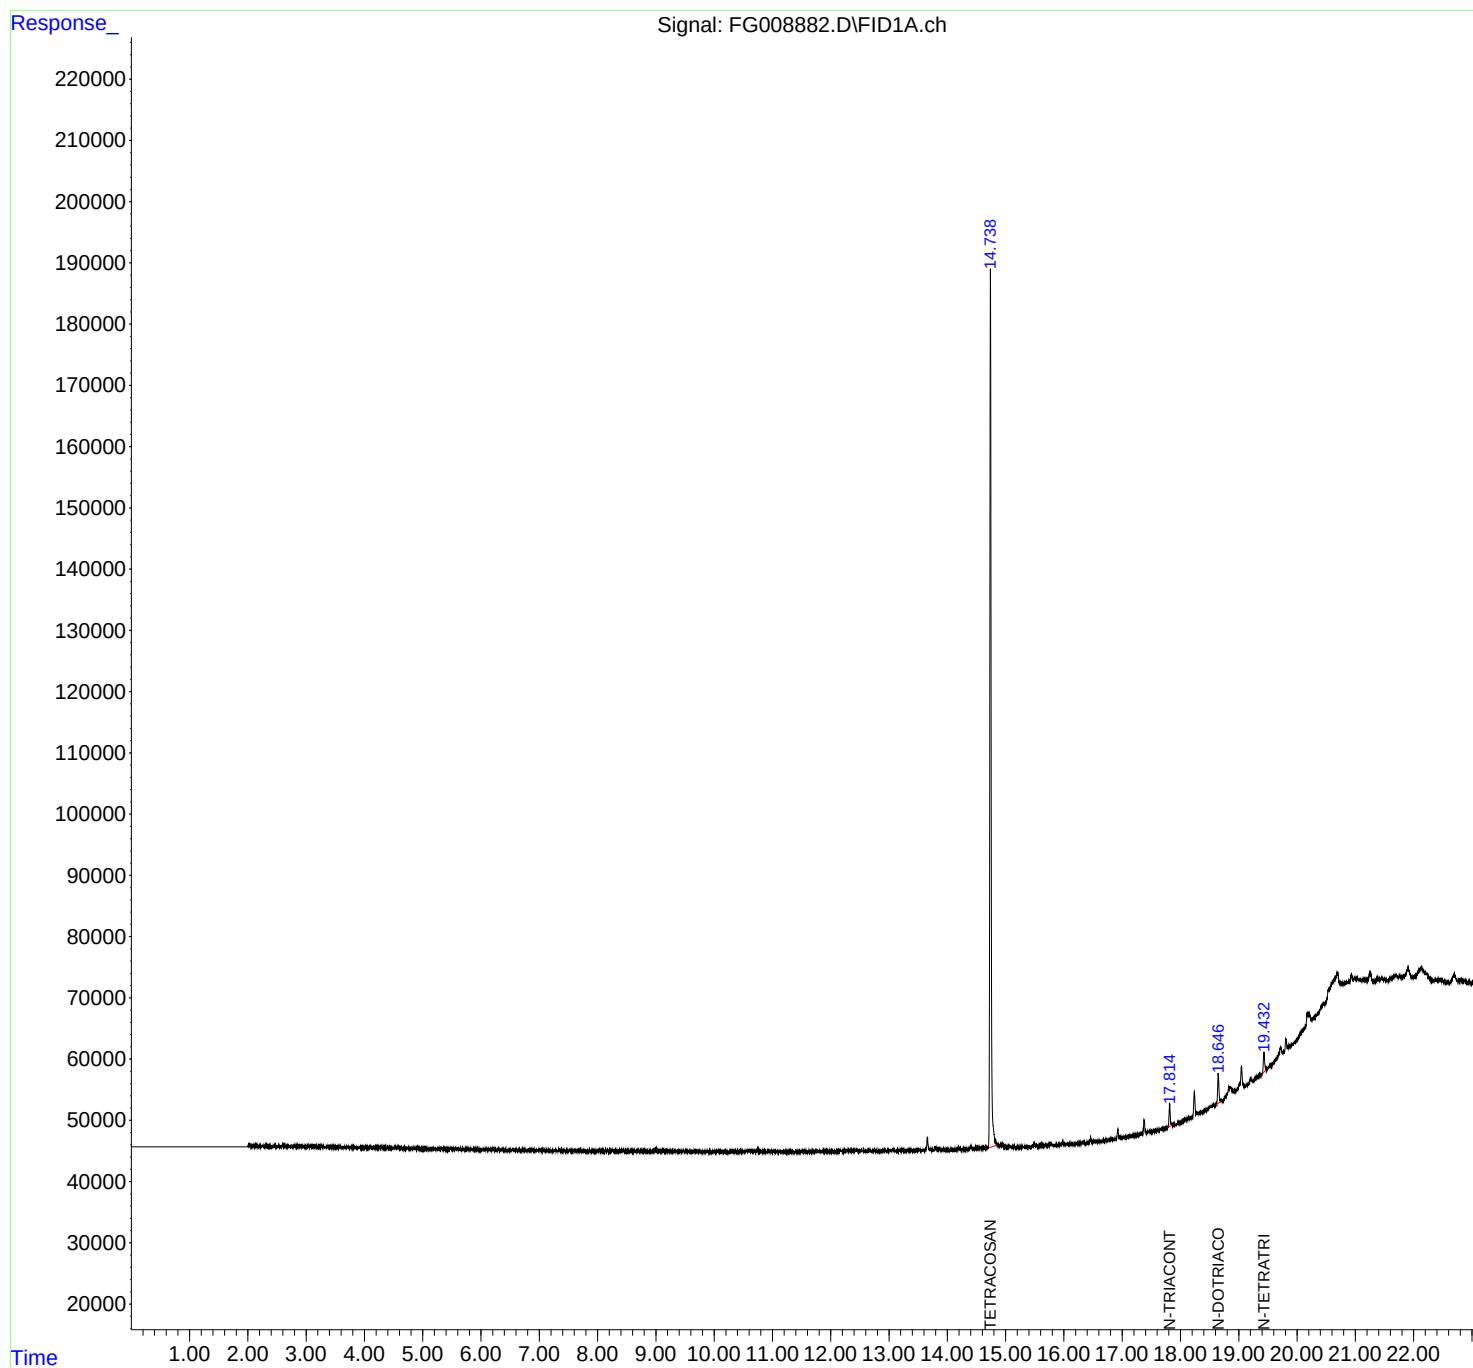


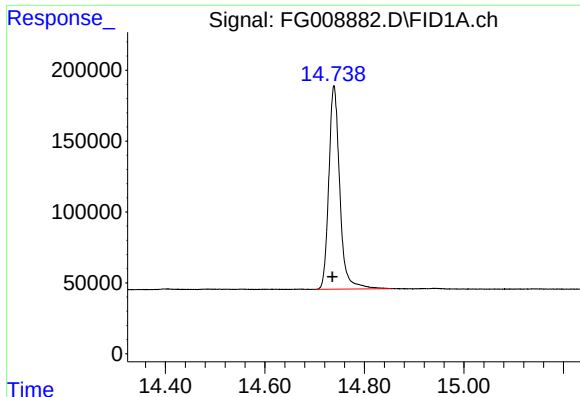

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.739 min
Delta R.T.: 0.003 min
Response: 2195139
Conc: 19.02 ug/ml

Instrument :
FID_G
ClientSampleId :

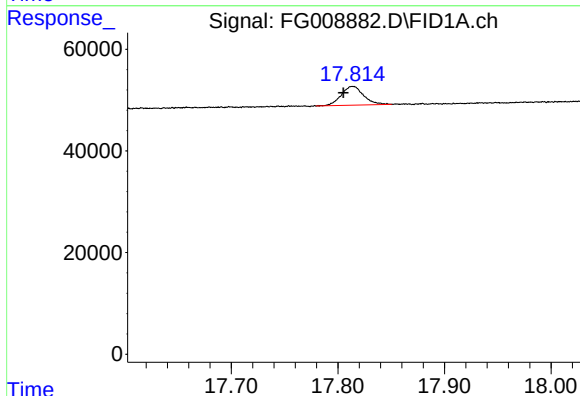


#13 N-TRIACONTANE

R.T.: 17.814 min
Delta R.T.: 0.009 min
Response: 53264
Conc: 0.47 ug/ml

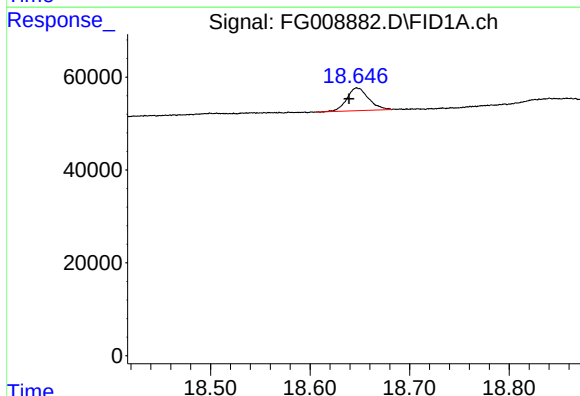

#14 N-DOTRIACONTANE

R.T.: 18.647 min
Delta R.T.: 0.008 min
Response: 73788
Conc: 0.70 ug/ml

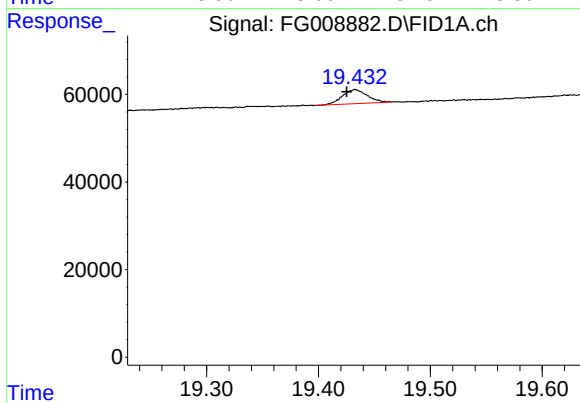

#15 N-TETRATRIACONTANE

R.T.: 19.433 min
Delta R.T.: 0.008 min
Response: 49147
Conc: 0.49 ug/ml