

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
Data File : FG008885.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2021 13:23
Operator : AJ\MA
Sample : PB139889BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:50:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	2294268	19.876 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.648	55603	0.524 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
Data File : FG008885.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2021 13:23
Operator : AJ\MA
Sample : PB139889BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:50:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

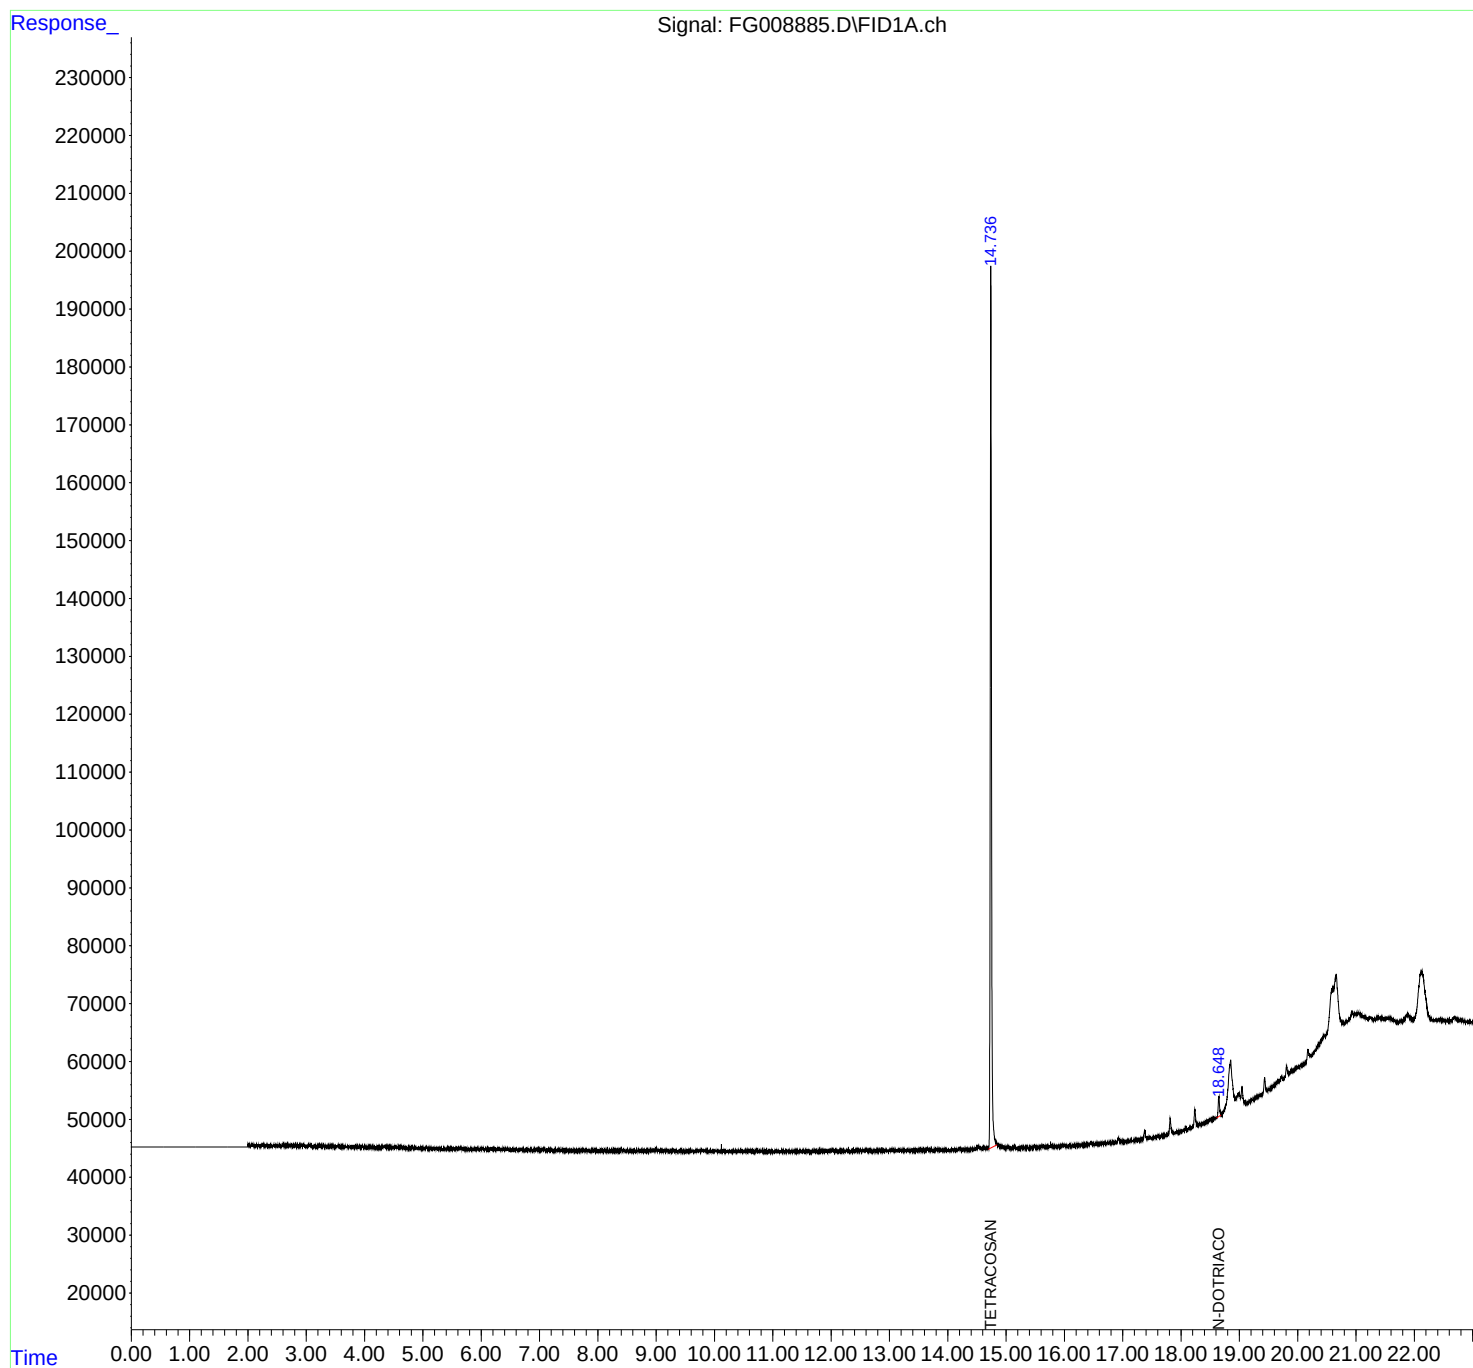


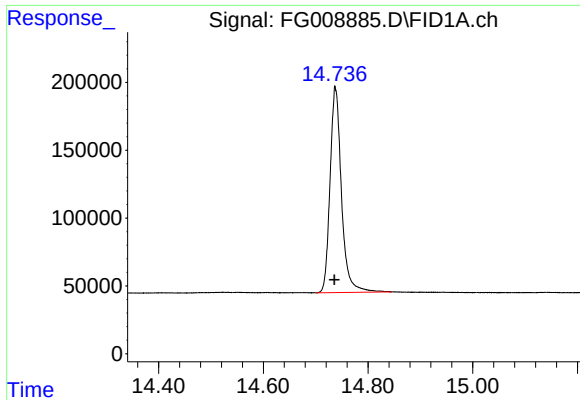

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: 0.001 min
Response: 2294268
Conc: 19.88 ug/ml

Instrument :
FID_G
ClientSampleId :

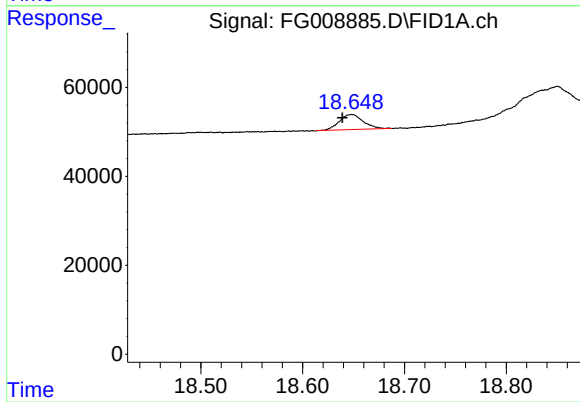

#14 N-DOTRIACONTANE

R.T.: 18.648 min
Delta R.T.: 0.009 min
Response: 55603
Conc: 0.52 ug/ml