

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
 Data File : FG008887.D
 Signal(s) : FID1A.ch
 Acq On : 15 Oct 2021 14:58
 Operator : AJ\MA
 Sample : PB139876BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 16 00:50:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
 Quant Title :
 QLast Update : Fri Oct 08 03:31:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	2322439	20.120 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.814	61639	0.543 ug/ml
14) N-DOTRIACONTANE	18.649	117639	1.109 ug/ml
15) N-TETRATRIACONTANE	19.434	62072	0.623 ug/ml
16) N-HEXATRIACONTANE	20.209	129107	1.398 ug/ml
18) N-TETRACONTANE	21.907	246007	2.763 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
Data File : FG008887.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2021 14:58
Operator : AJ\MA
Sample : PB139876BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:50:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

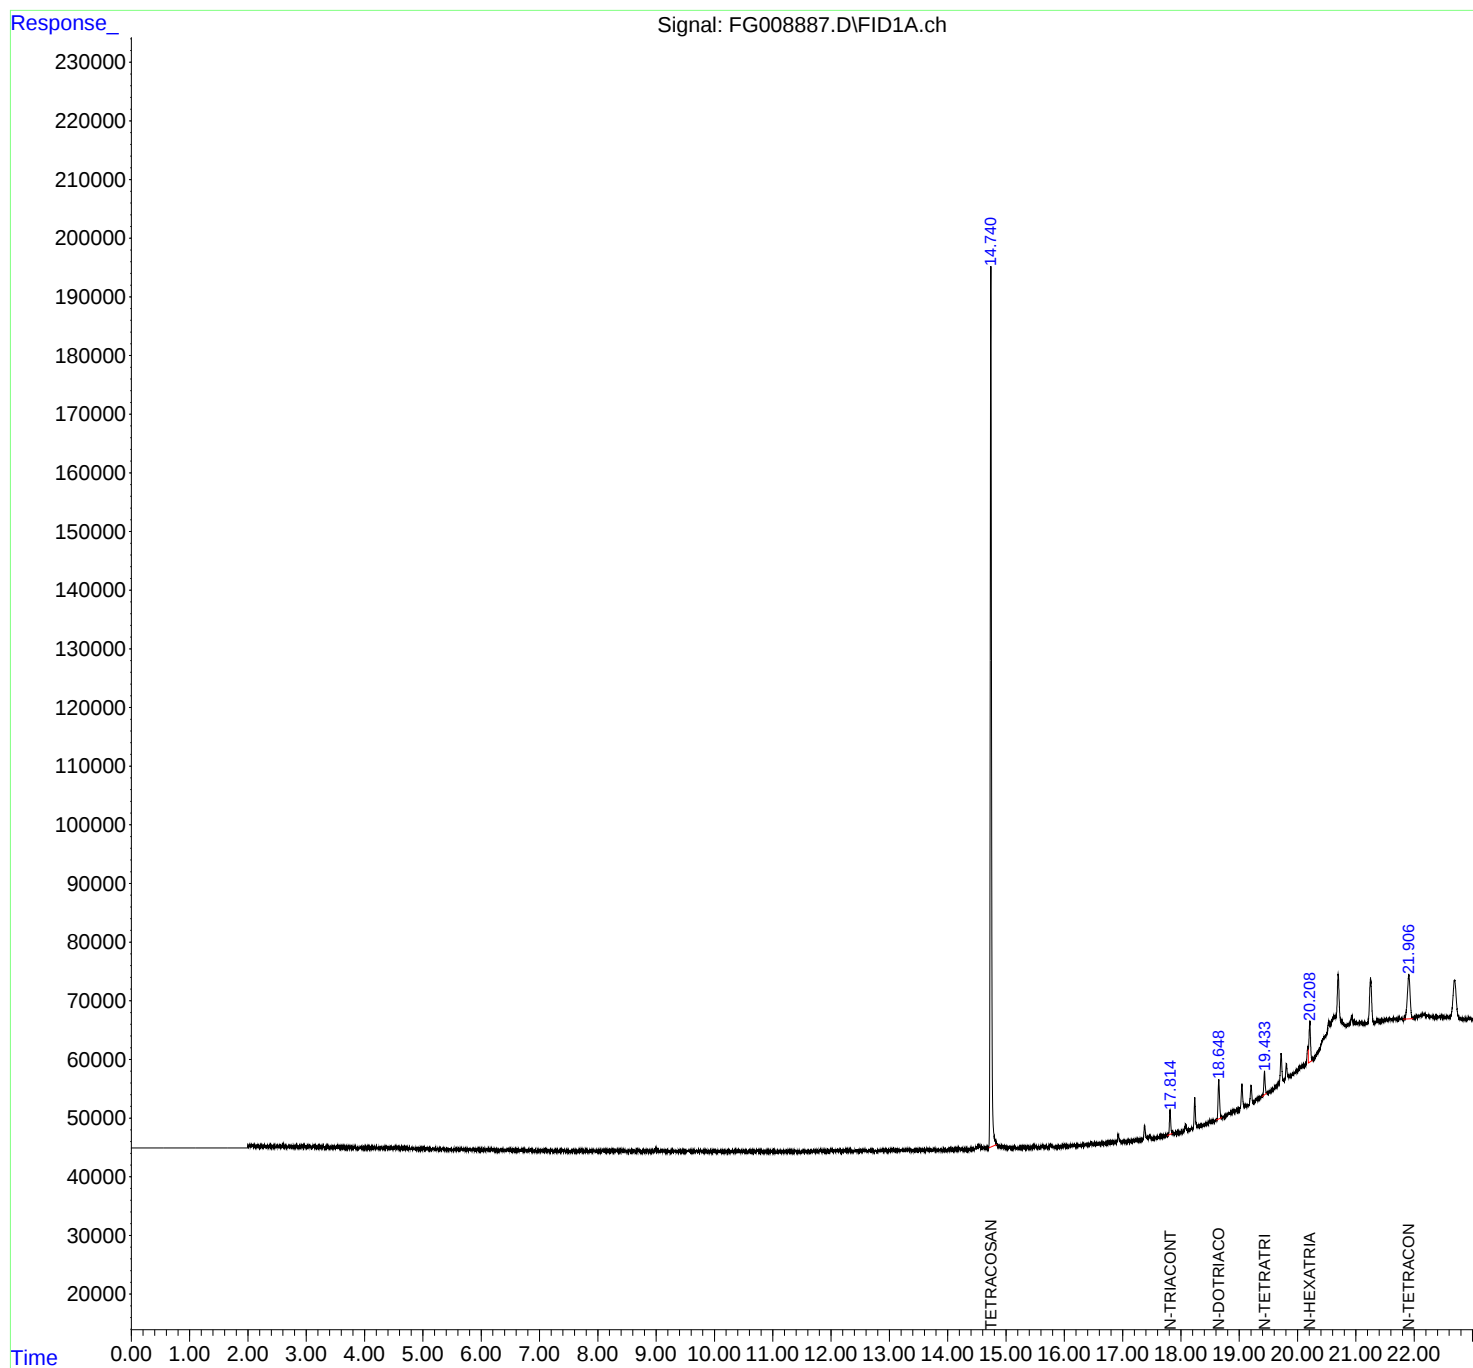


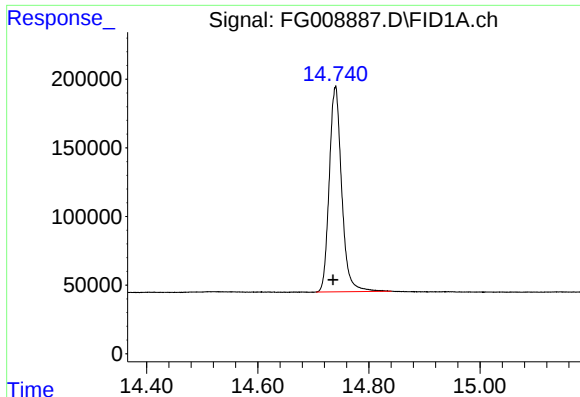

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.740 min
Delta R.T.: 0.005 min
Response: 2322439
Conc: 20.12 ug/ml

Instrument :
FID_G
ClientSampleId :

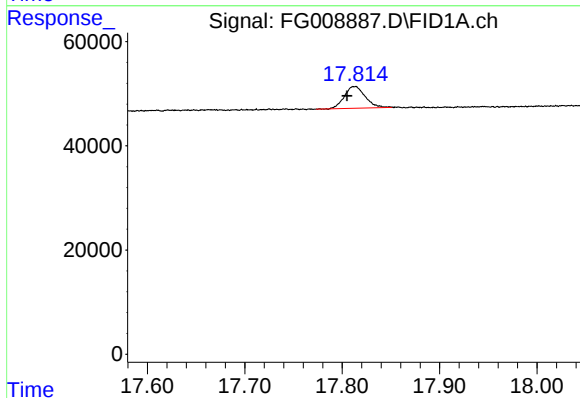


#13 N-TRIACONTANE

R.T.: 17.814 min
Delta R.T.: 0.009 min
Response: 61639
Conc: 0.54 ug/ml

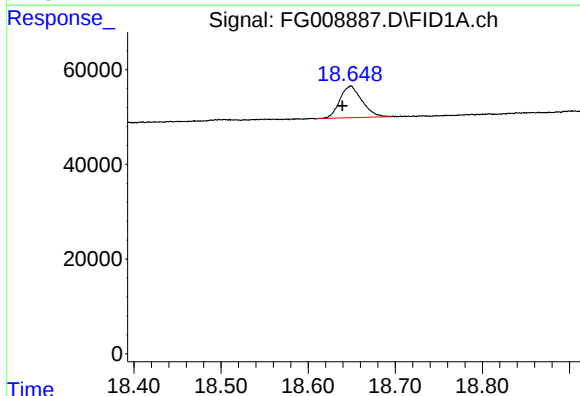


#14 N-DOTRIACONTANE

R.T.: 18.649 min
Delta R.T.: 0.010 min
Response: 117639
Conc: 1.11 ug/ml

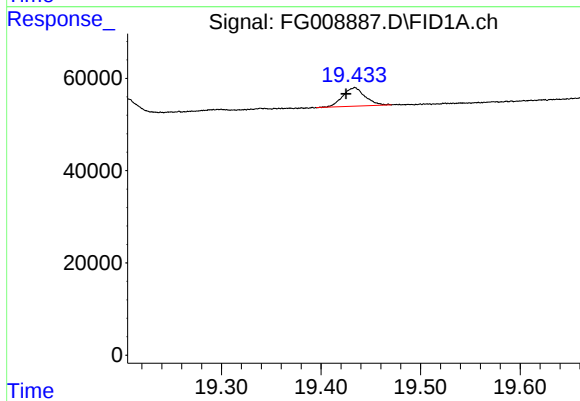

#15 N-TETRATRIACONTANE


R.T.: 19.434 min
Delta R.T.: 0.009 min
Response: 62072
Conc: 0.62 ug/ml

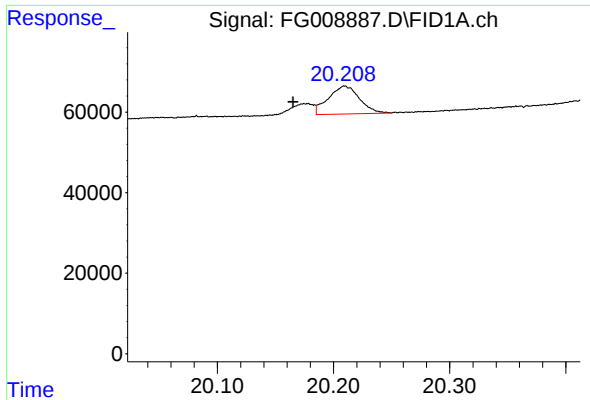

#16 N-HEXATRIACONTANE

R.T.: 20.209 min
Delta R.T.: 0.044 min
Response: 129107
Conc: 1.40 ug/ml

Instrument :
FID_G
ClientSampleId :

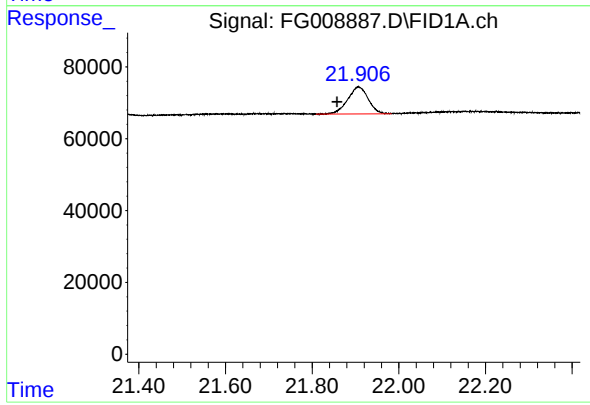

#18 N-TETRACONTANE

R.T.: 21.907 min
Delta R.T.: 0.049 min
Response: 246007
Conc: 2.76 ug/ml