

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
Data File : FG008884.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2021 10:49
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 16 00:49:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.467	3311387	23.484 ug/ml
12)	N-OCTACOSANE	16.921	3164009	26.552 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
Data File : FG008884.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2021 10:49
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 16 00:49:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

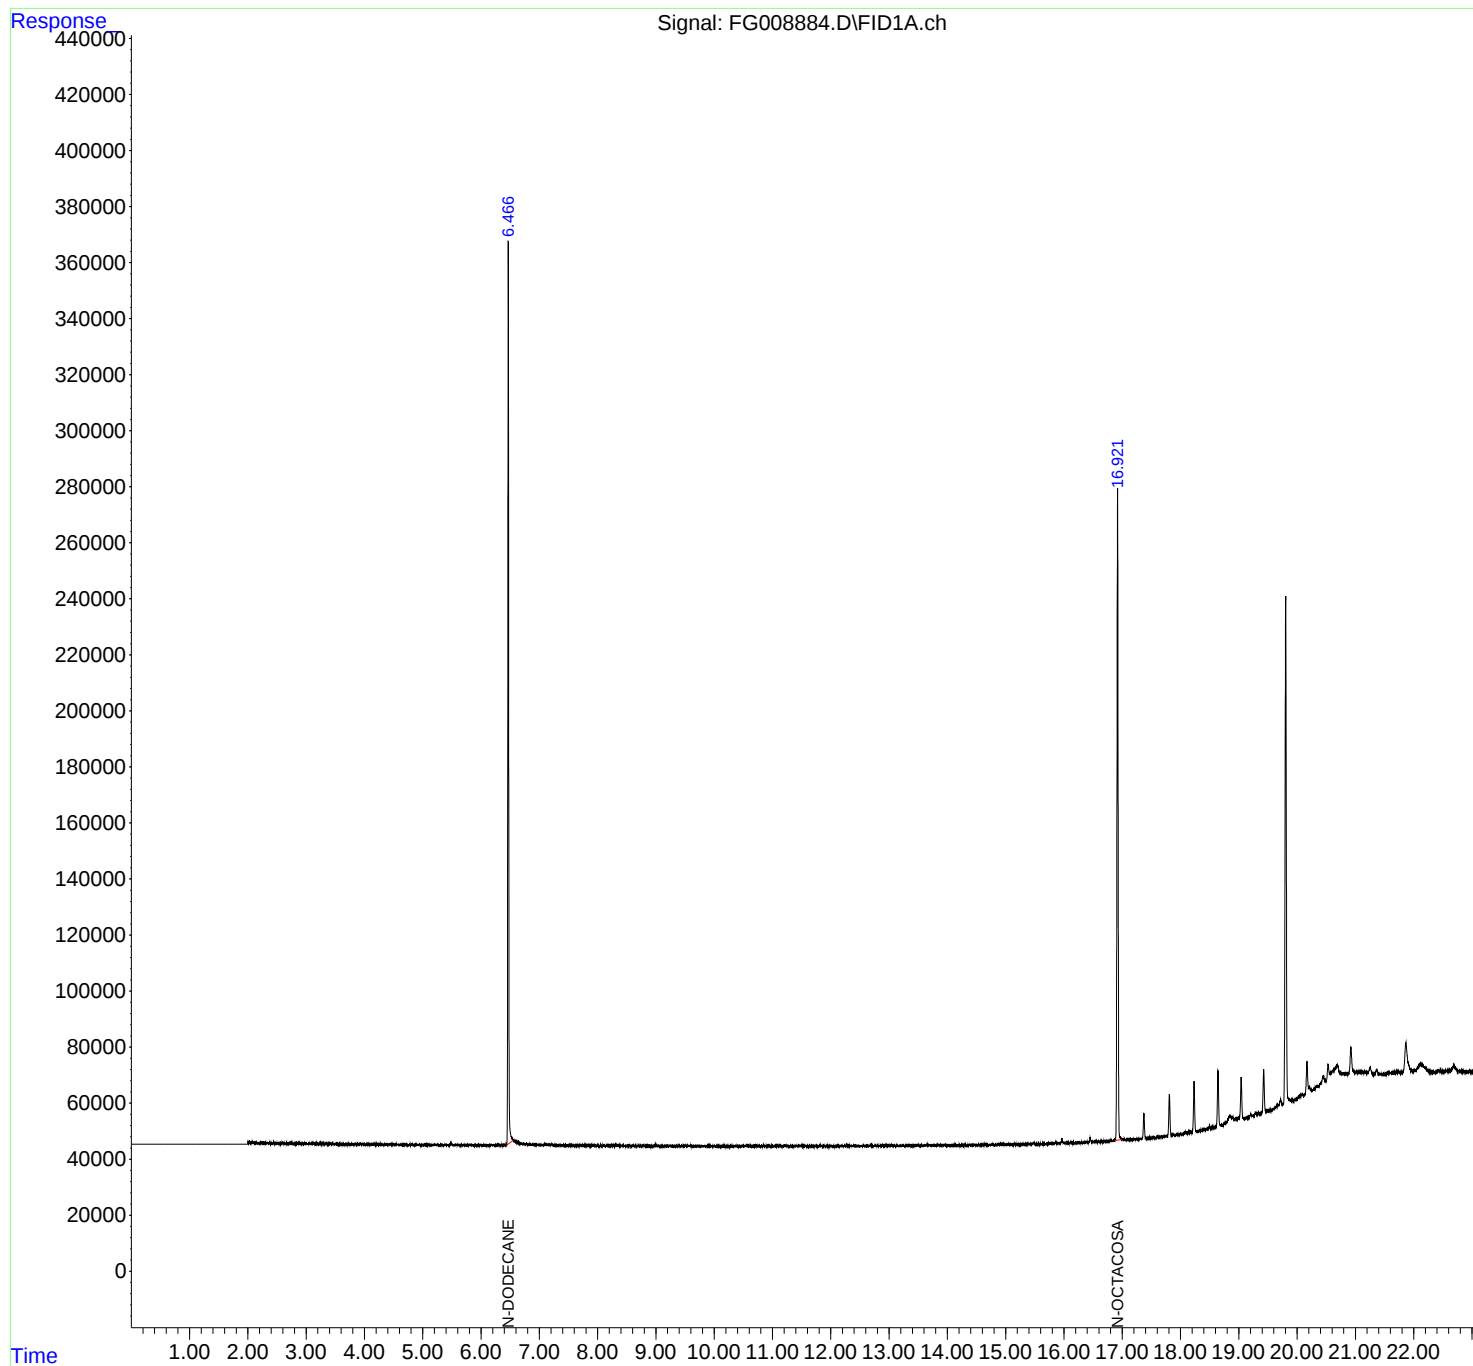


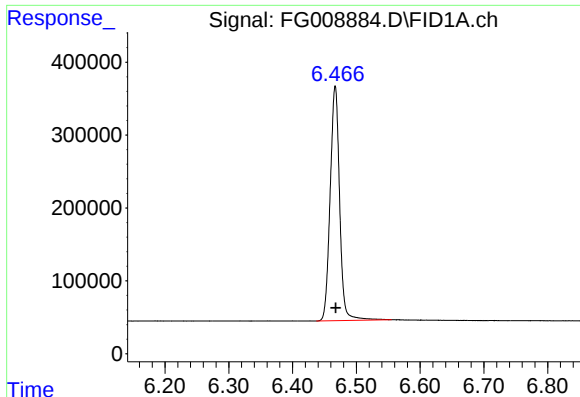

#3 N-DODECANE


R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 3311387
Conc: 23.48 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

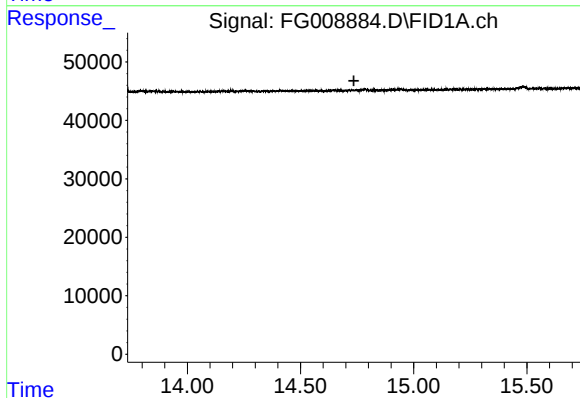

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.736 min
Response: 0
Conc: N.D.

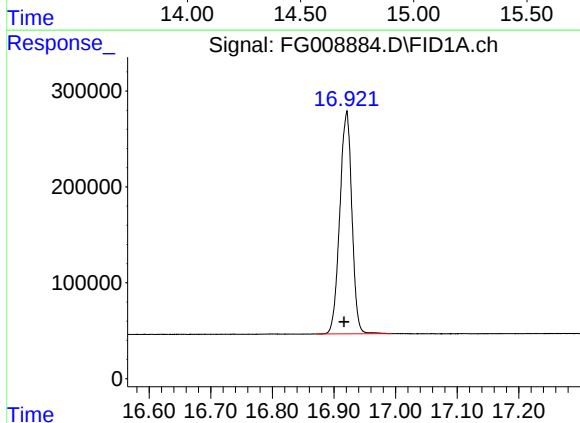

#12 N-OCTACOSANE

R.T.: 16.921 min
Delta R.T.: 0.005 min
Response: 3164009
Conc: 26.55 ug/ml