

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
Data File : FG008905.D
Signal(s) : FID1A.ch
Acq On : 16 Oct 2021 00:21
Operator : AJ\MA
Sample : M4089-08 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 16 00:55:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.739	408134	3.536 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Instrument :
FID_G
ClientSampleId :
20-SB-1-20211005-7.5-8.0

Manual Integrations
APPROVED

mohammad
10/18/2021 4:37:45 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101521\
Data File : FG008905.D
Signal(s) : FID1A.ch
Acq On : 16 Oct 2021 00:21
Operator : AJ\MA
Sample : M4089-08 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
20-SB-1-20211005-7.5-8.0


Manual Integrations
APPROVED

mohammad
10/18/2021 4:37:45 PM

Integration File: autoint1.e
Quant Time: Oct 16 00:55:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

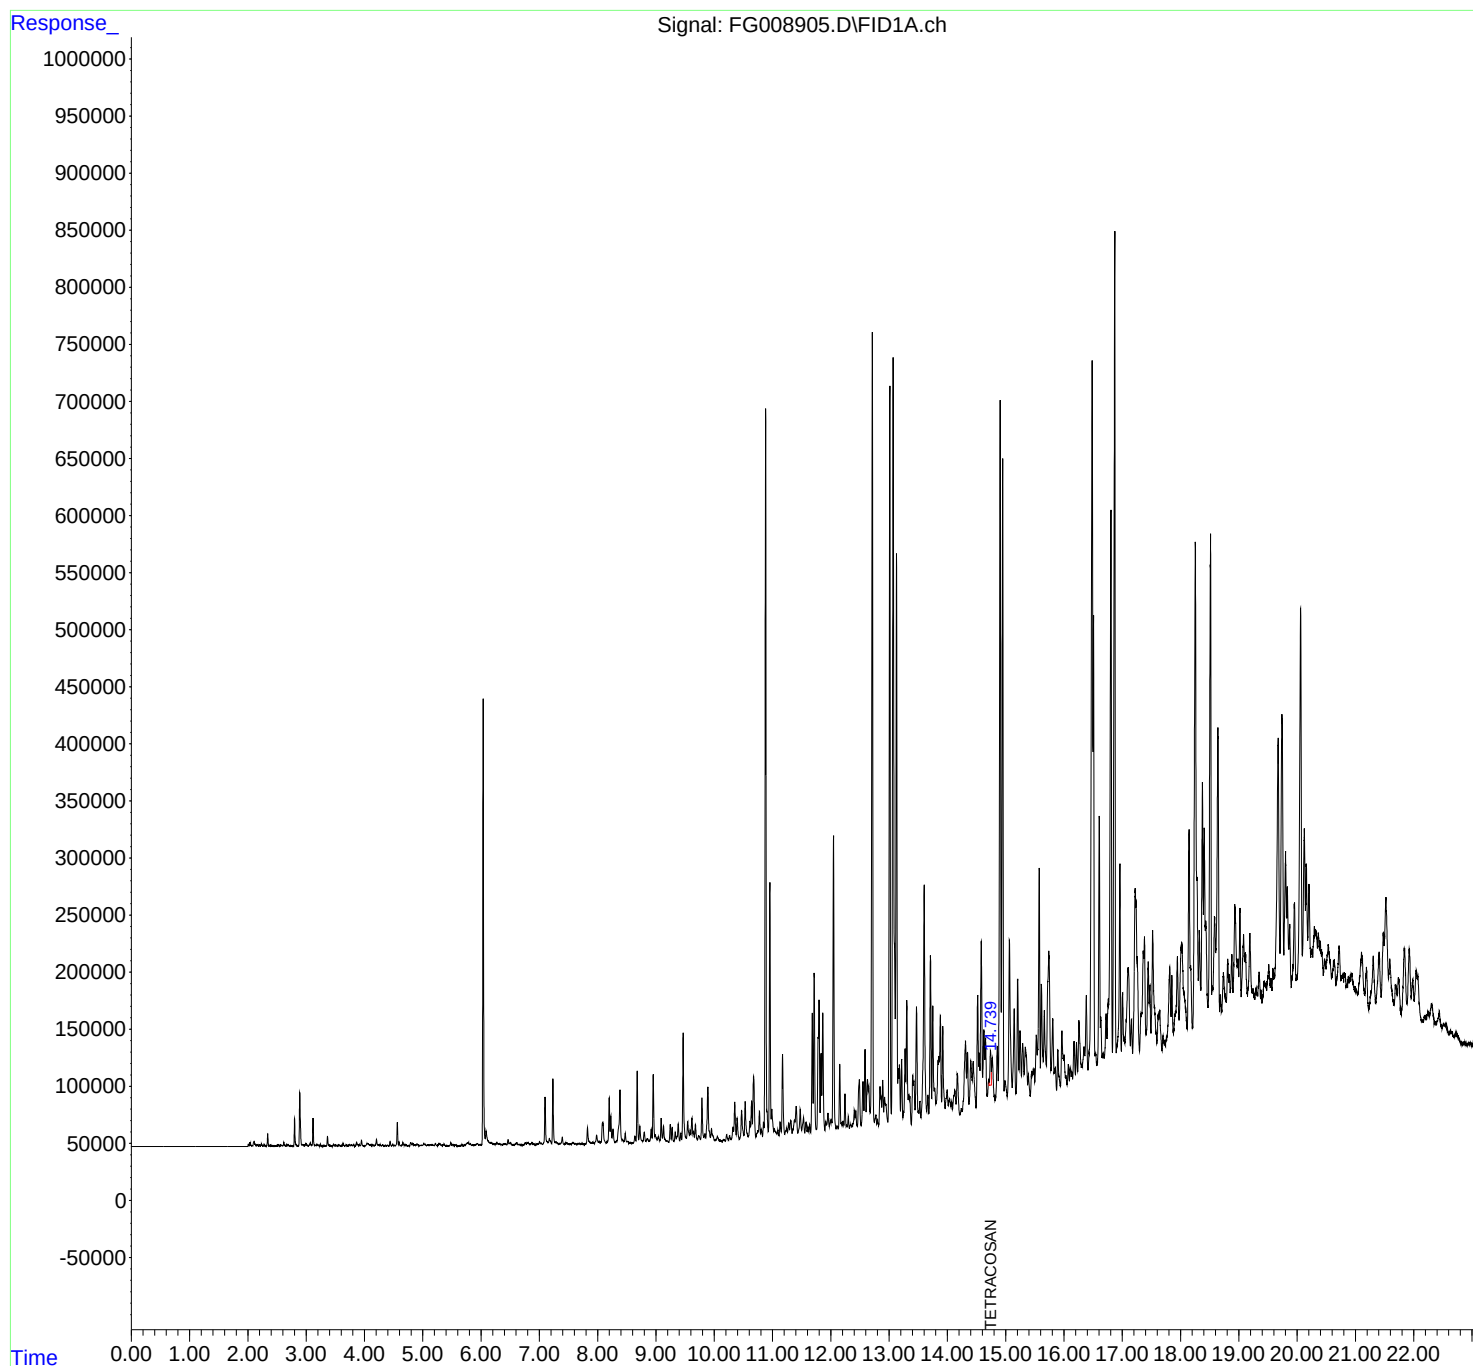

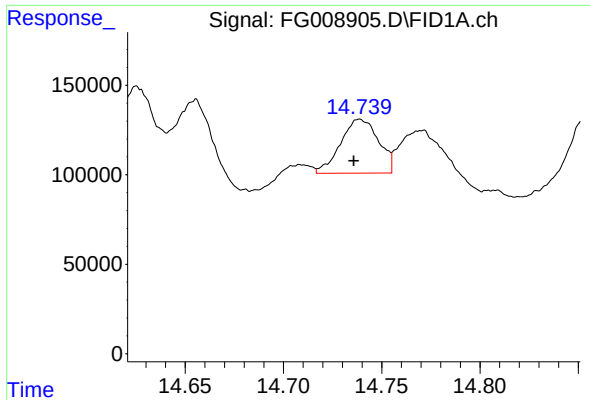

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.739 min
Delta R.T.: 0.003 min
Response: 408134
Conc: 3.54 ug/ml m

Instrument :
FID_G
ClientSampleId :
20-SB-1-20211005-7.5-8.0

Manual Integrations
APPROVED

mohammad
10/18/2021 4:37:45 PM