

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101818\
Data File : FG002616.D
Signal(s) : FID1A.ch
Acq On : 18 Oct 2018 16:12
Operator : AJ\SJ
Sample : J5202-05 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 18 23:40:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.759	122006	1.063 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.829	165310	1.314 ug/ml
16) N-HEXATRIACONTANE	20.206	39906	0.360 ug/ml


(f)=RT Delta > 1/2 Window

(m)=manual int.

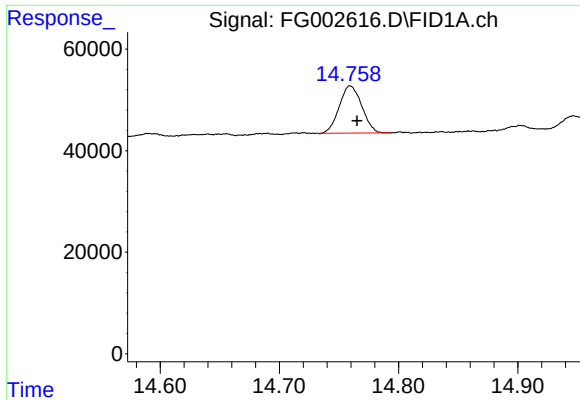


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.759 min
Delta R.T.: -0.006 min
Response: 122006
Conc: 1.06 ug/ml

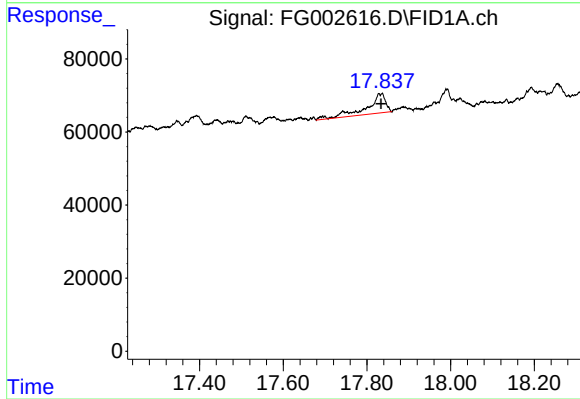

#13 N-TRIACONTANE

R.T.: 17.829 min
Delta R.T.: -0.005 min
Response: 165310
Conc: 1.31 ug/ml

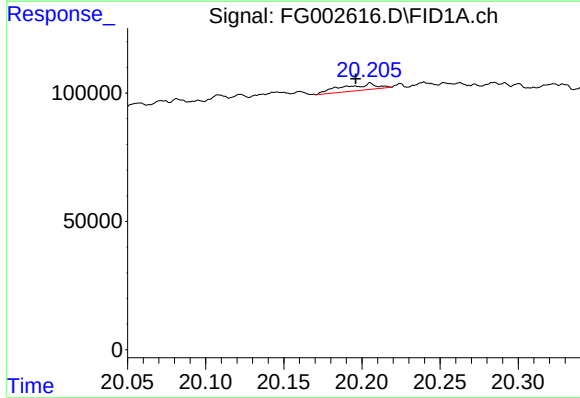

#16 N-HEXATRIACONTANE

R.T.: 20.206 min
Delta R.T.: 0.010 min
Response: 39906
Conc: 0.36 ug/ml