

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101818\
 Data File : FG002618.D
 Signal(s) : FID1A.ch
 Acq On : 18 Oct 2018 17:12
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 18 23:40:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:36:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.764	1833993	15.978 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.831	96223	0.765 ug/ml
14)	N-DOTRIACONTANE	18.669	121789	0.992 ug/ml
15)	N-TETRATRIACONTANE	19.452	108490	0.909 ug/ml
16)	N-HEXATRIACONTANE	20.192	116405	1.049 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101818\
Data File : FG002618.D
Signal(s) : FID1A.ch
Acq On : 18 Oct 2018 17:12
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 18 23:40:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

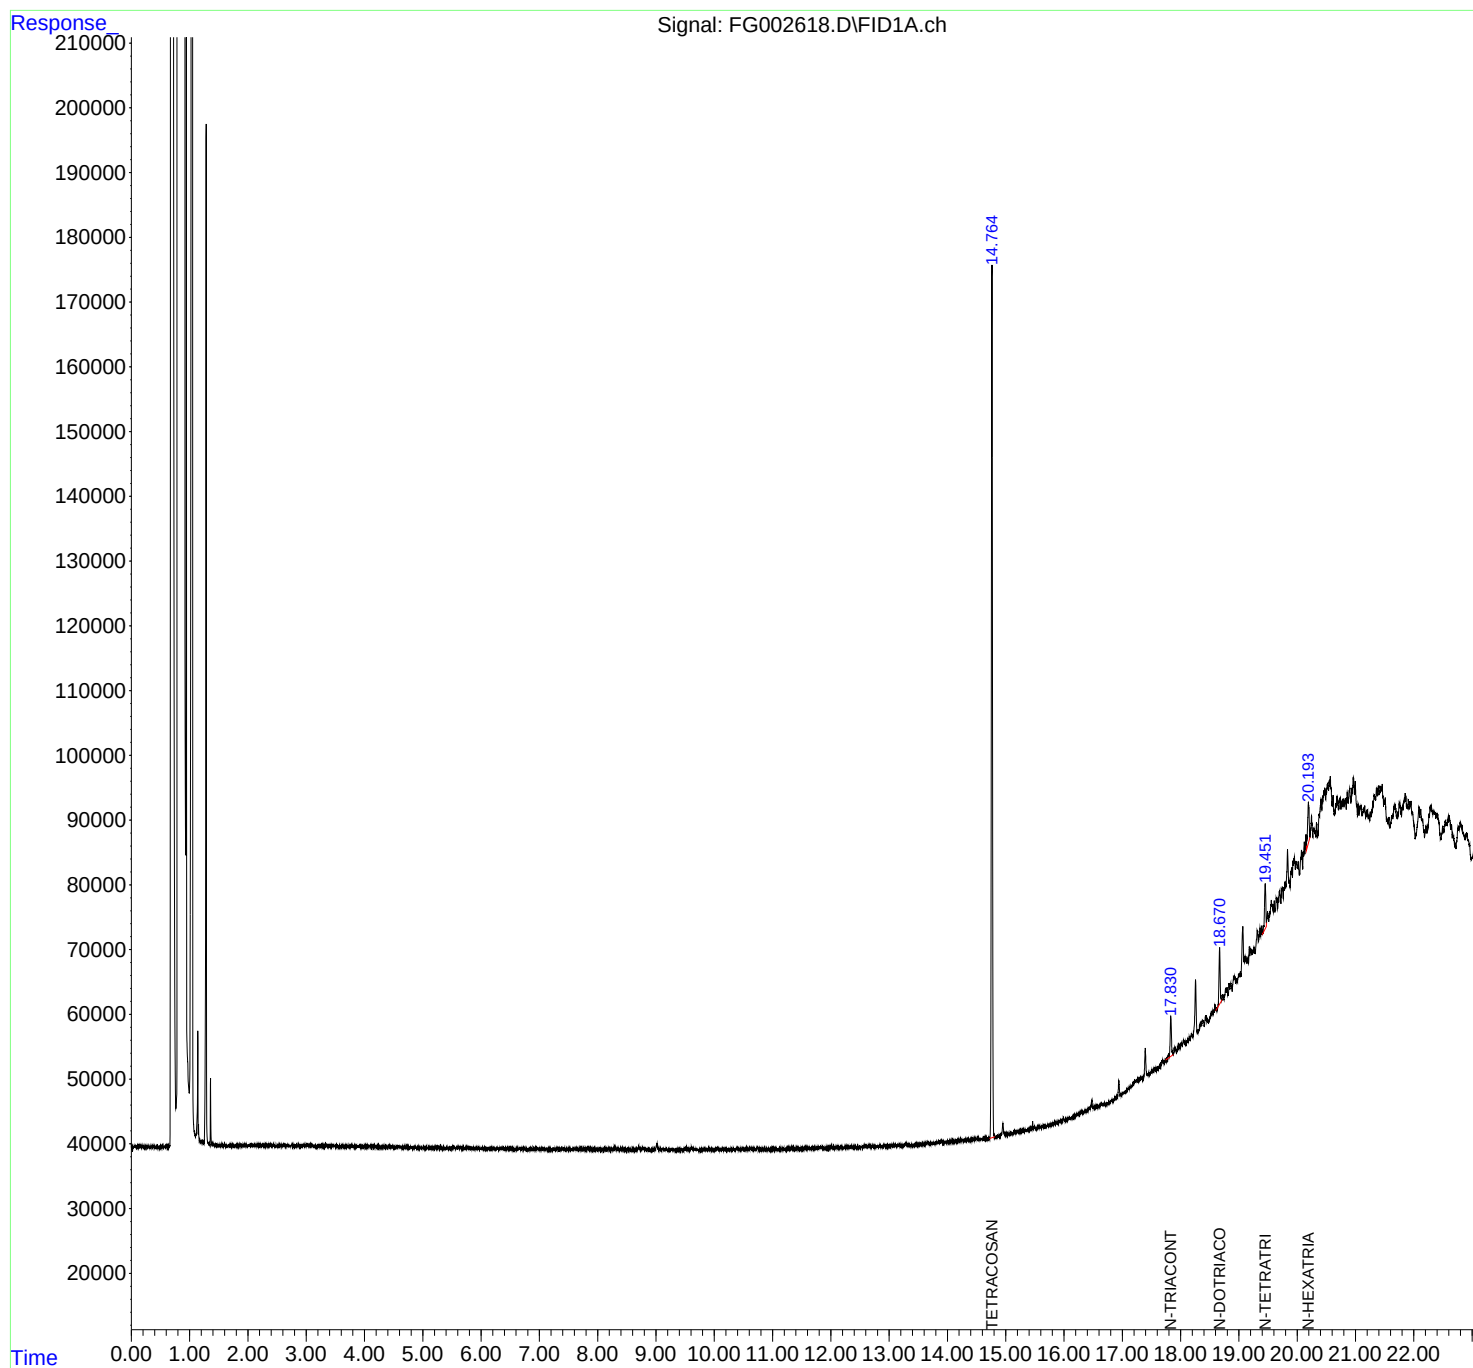

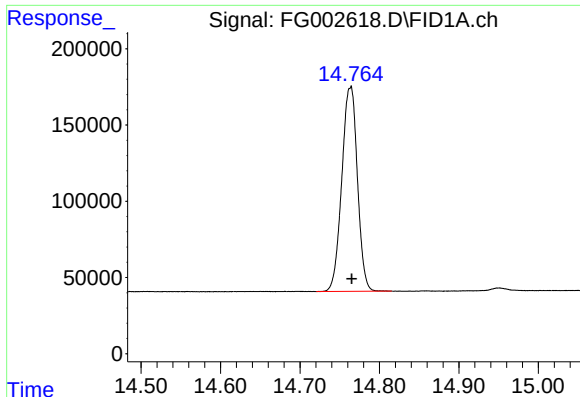


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.764 min
Delta R.T.: -0.002 min
Response: 1833993
Conc: 15.98 ug/ml

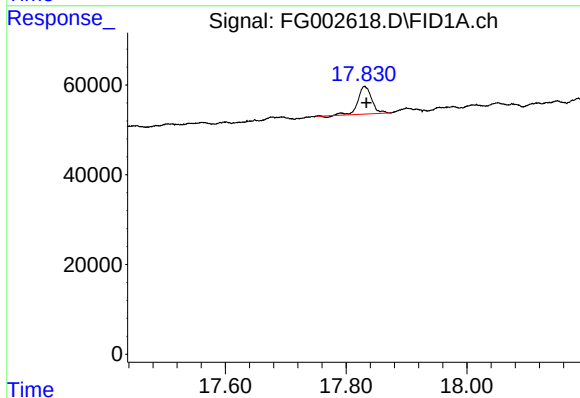


#13 N-TRIACONTANE

R.T.: 17.831 min
Delta R.T.: -0.003 min
Response: 96223
Conc: 0.76 ug/ml

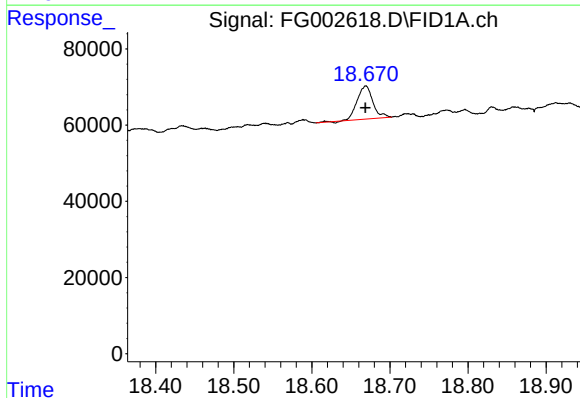


#14 N-DOTRIACONTANE

R.T.: 18.669 min
Delta R.T.: 0.000 min
Response: 121789
Conc: 0.99 ug/ml

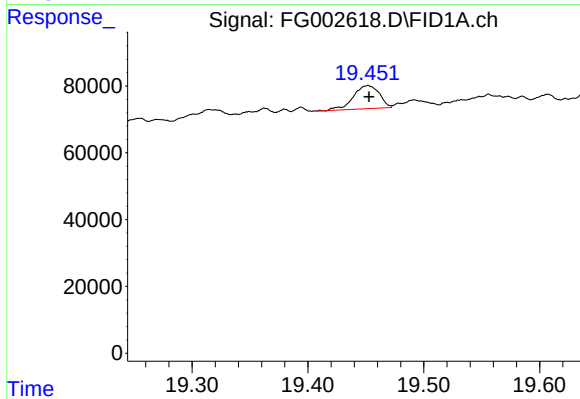

#15 N-TETRATRIACONTANE

R.T.: 19.452 min
Delta R.T.: 0.000 min
Response: 108490
Conc: 0.91 ug/ml

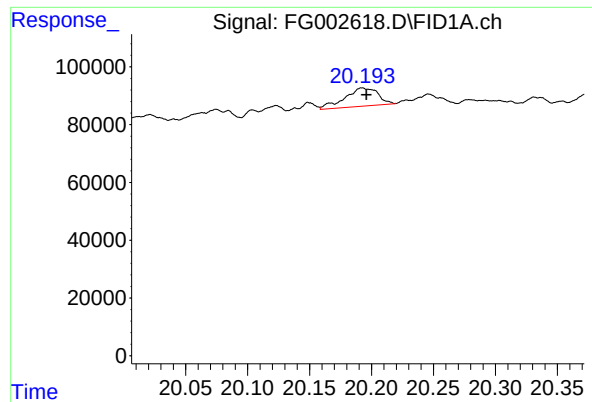

#16 N-HEXATRIACONTANE

R.T.: 20.192 min
Delta R.T.: -0.003 min
Response: 116405
Conc: 1.05 ug/ml