

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101818\
 Data File : FG002619.D
 Signal(s) : FID1A.ch
 Acq On : 18 Oct 2018 17:42
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Oct 18 23:40:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:36:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.766	5662792	49.335 ug/ml
Target Compounds			
2) N-DECANE	4.463	6855941	52.620 ug/ml
3) N-DODECANE	6.494	6870018	52.057 ug/ml
4) N-TETRADECANE	8.295	6855525	51.416 ug/ml
5) N-HEXADECANE	9.901	6831274	50.924 ug/ml
6) N-OCTADECANE	11.348	6796334	50.465 ug/ml
7) N-EICOSANE	12.662	6676738	50.055 ug/ml
8) N-DOCOSANE	13.864	6581511	49.877 ug/ml
10) N-TETRACOSANE	14.971	6491591	49.935 ug/ml
11) N-HEXACOSANE	15.994	6461012	50.297 ug/ml
12) N-OCTACOSANE	16.947	6541090	51.592 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101818\
Data File : FG002619.D
Signal(s) : FID1A.ch
Acq On : 18 Oct 2018 17:42
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Oct 18 23:40:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

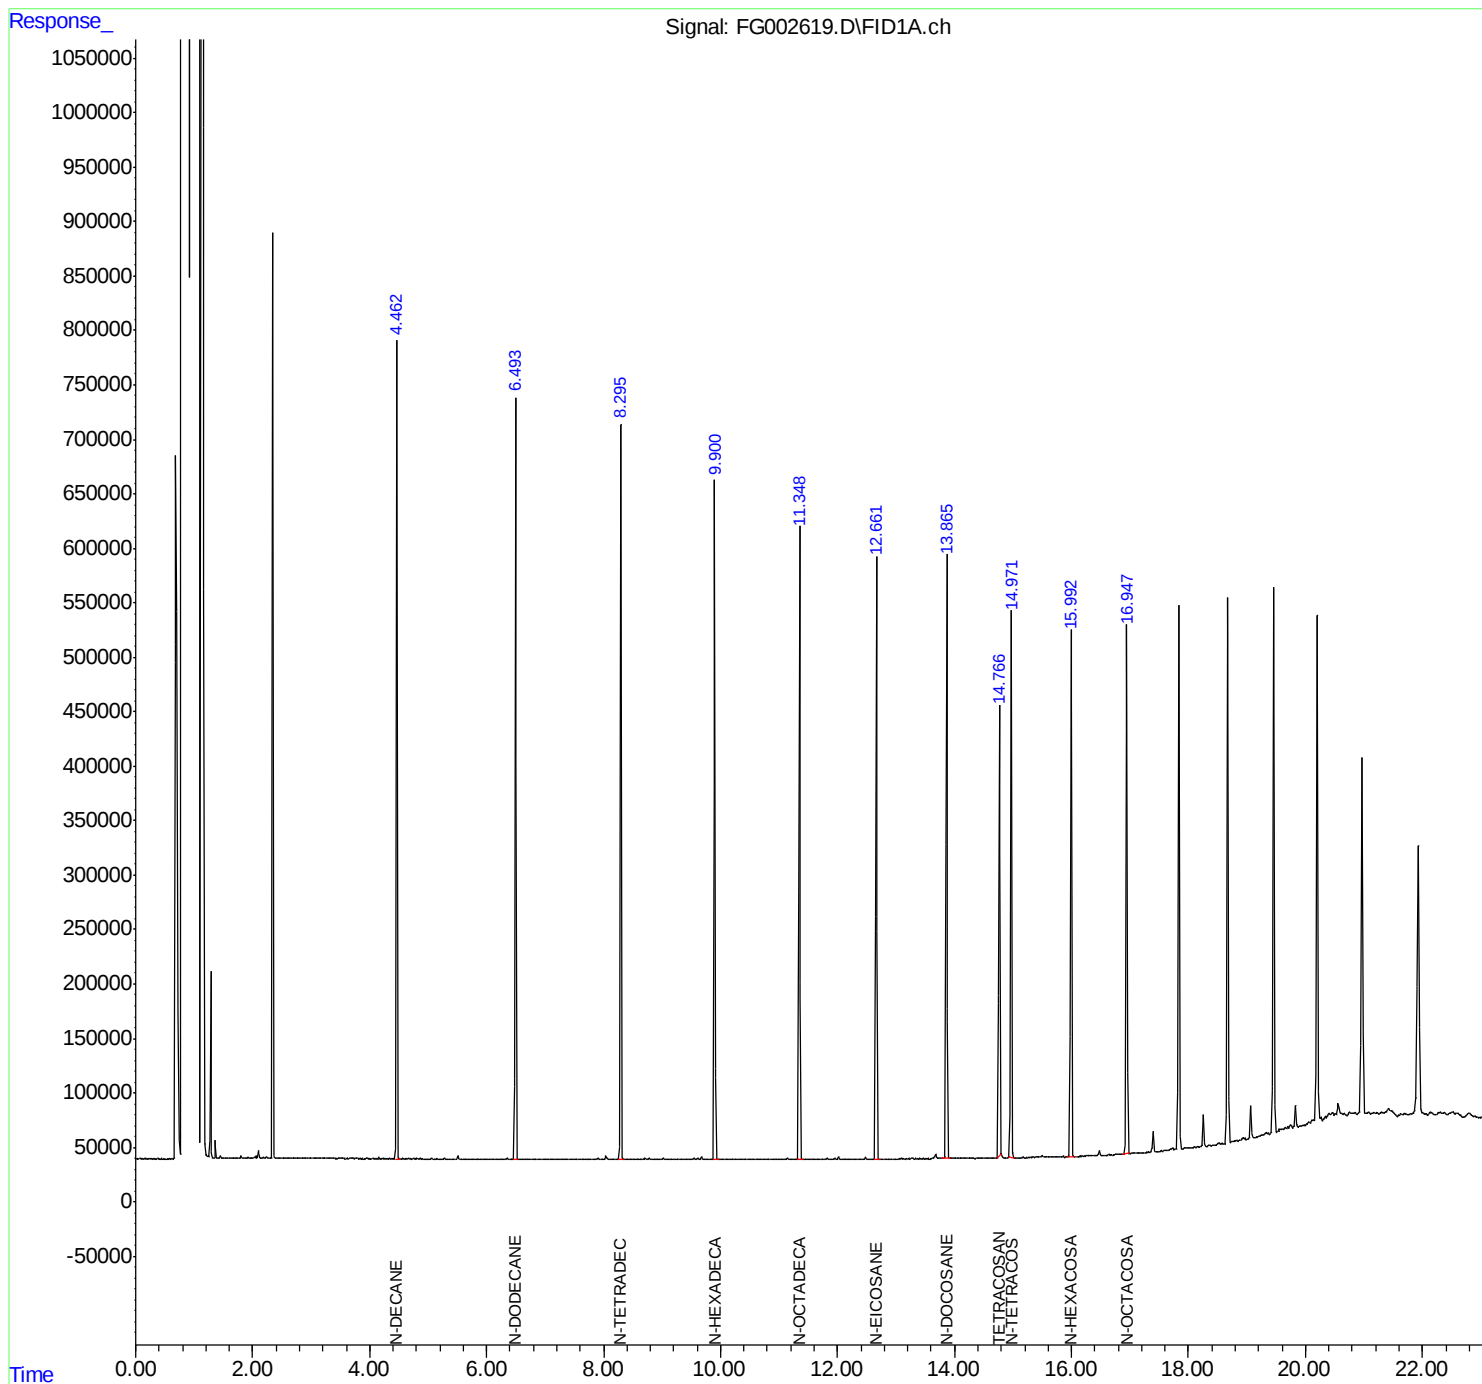

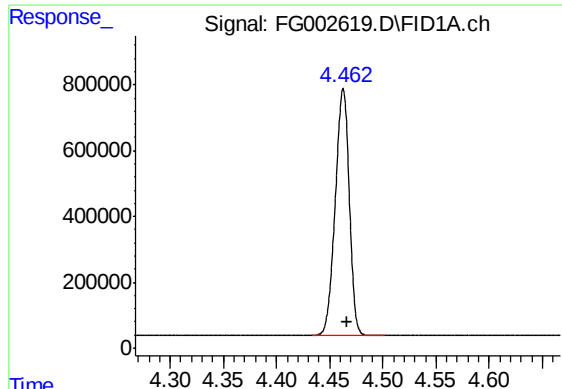


#2 N-DECANE

R.T.: 4.463 min
Delta R.T.: -0.004 min
Response: 6855941
Conc: 52.62 ug/ml

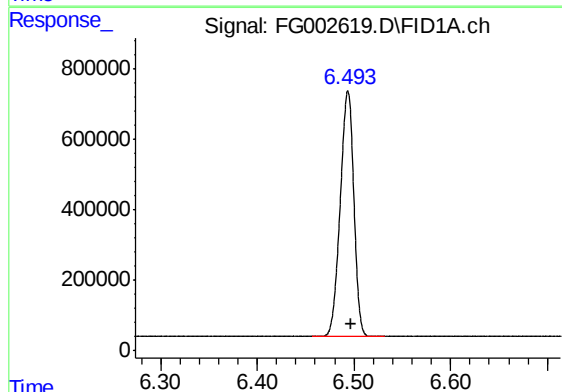


#3 N-DODECANE

R.T.: 6.494 min
Delta R.T.: -0.004 min
Response: 6870018
Conc: 52.06 ug/ml

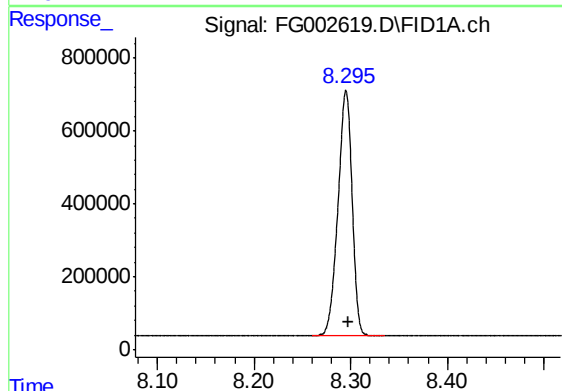


#4 N-TETRADECANE

R.T.: 8.295 min
Delta R.T.: -0.003 min
Response: 6855525
Conc: 51.42 ug/ml

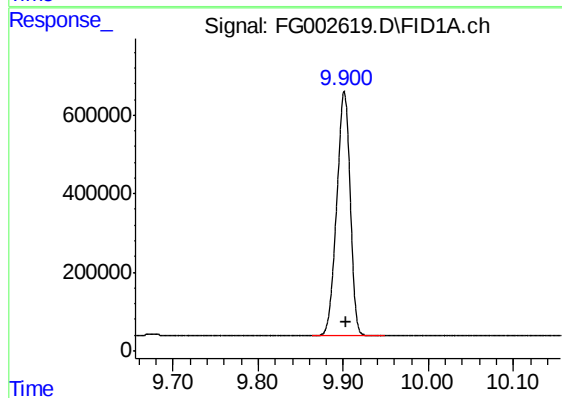


#5 N-HEXADECANE

R.T.: 9.901 min
Delta R.T.: -0.003 min
Response: 6831274
Conc: 50.92 ug/ml

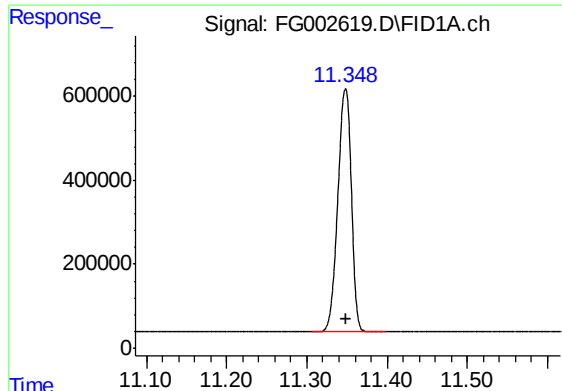


#6 N-OCTADECANE

R.T.: 11.348 min
Delta R.T.: -0.001 min
Response: 6796334
Conc: 50.46 ug/ml

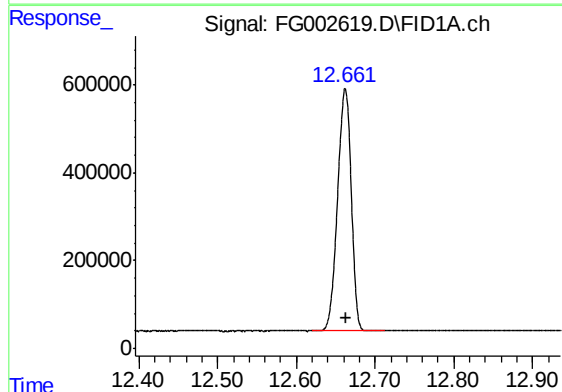


#7 N-EICOSANE

R.T.: 12.662 min
Delta R.T.: 0.000 min
Response: 6676738
Conc: 50.05 ug/ml

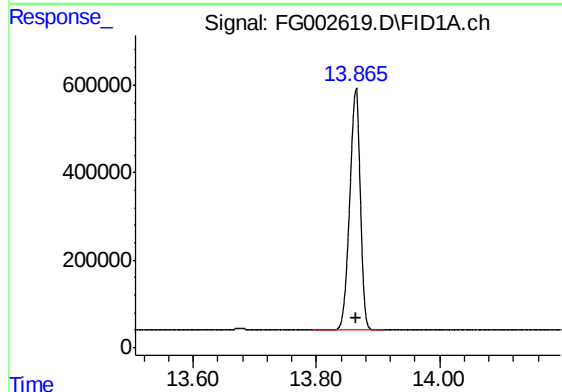


#8 N-DOCOSANE

R.T.: 13.864 min
Delta R.T.: 0.000 min
Response: 6581511
Conc: 49.88 ug/ml

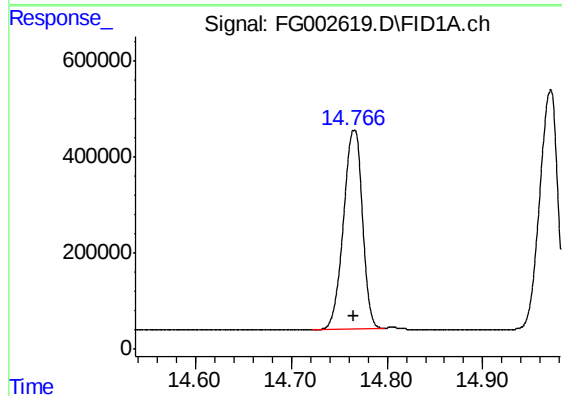


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.766 min
Delta R.T.: 0.000 min
Response: 5662792
Conc: 49.34 ug/ml

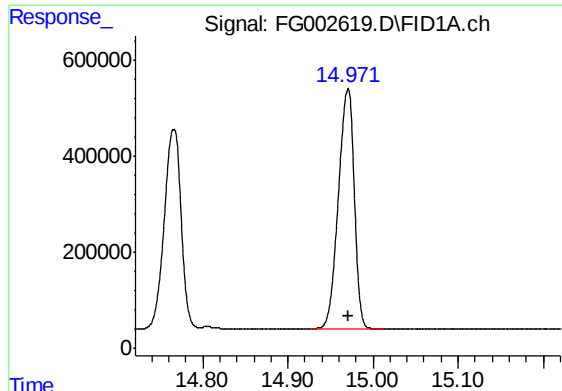


#10 N-TETRACOSANE

R.T.: 14.971 min
Delta R.T.: 0.000 min
Response: 6491591
Conc: 49.93 ug/ml

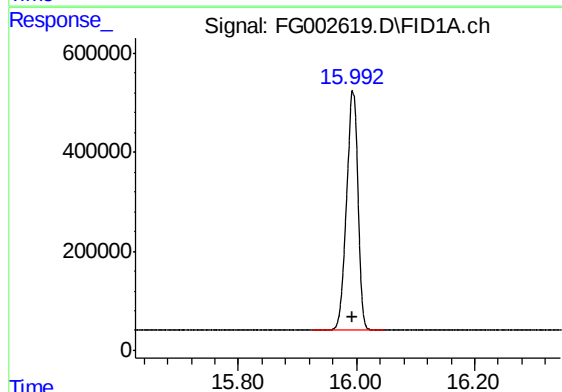

#11 N-HEXACOSANE

R.T.: 15.994 min
Delta R.T.: 0.000 min
Response: 6461012
Conc: 50.30 ug/ml

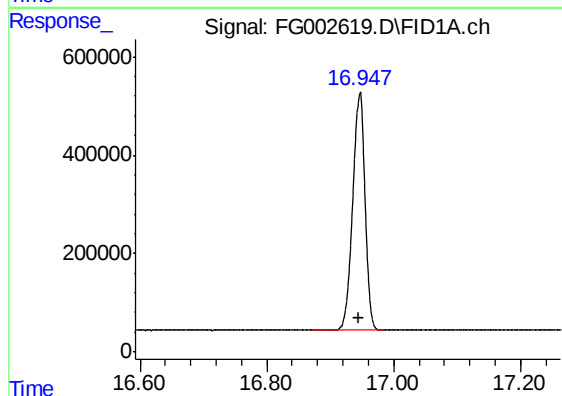

#12 N-OCTACOSANE

R.T.: 16.947 min
Delta R.T.: 0.002 min
Response: 6541090
Conc: 51.59 ug/ml