

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101821\
 Data File : FG008932.D
 Signal(s) : FID1A.ch
 Acq On : 18 Oct 2021 21:49
 Operator : AJ\MA
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Oct 19 00:26:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
 Quant Title :
 QLast Update : Fri Oct 08 03:31:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	4964917	43.013 ug/ml
Target Compounds			
2) N-DECANE	4.439	6697136	48.004 ug/ml
3) N-DODECANE	6.467	6677814	47.359 ug/ml
4) N-TETRADECANE	8.268	6553505	46.488 ug/ml
5) N-HEXADECANE	9.874	6351992	45.359 ug/ml
6) N-OCTADECANE	11.320	6285390	44.475 ug/ml
7) N-EICOSANE	12.634	6092834	43.688 ug/ml
8) N-DOCOSANE	13.837	5821597	43.161 ug/ml
10) N-TETRACOSANE	14.943	5636069	42.923 ug/ml
11) N-HEXACOSANE	15.968	5410723	43.222 ug/ml
12) N-OCTACOSANE	16.919	5278496	44.296 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101821\
Data File : FG008932.D
Signal(s) : FID1A.ch
Acq On : 18 Oct 2021 21:49
Operator : AJ\MA
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Oct 19 00:26:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

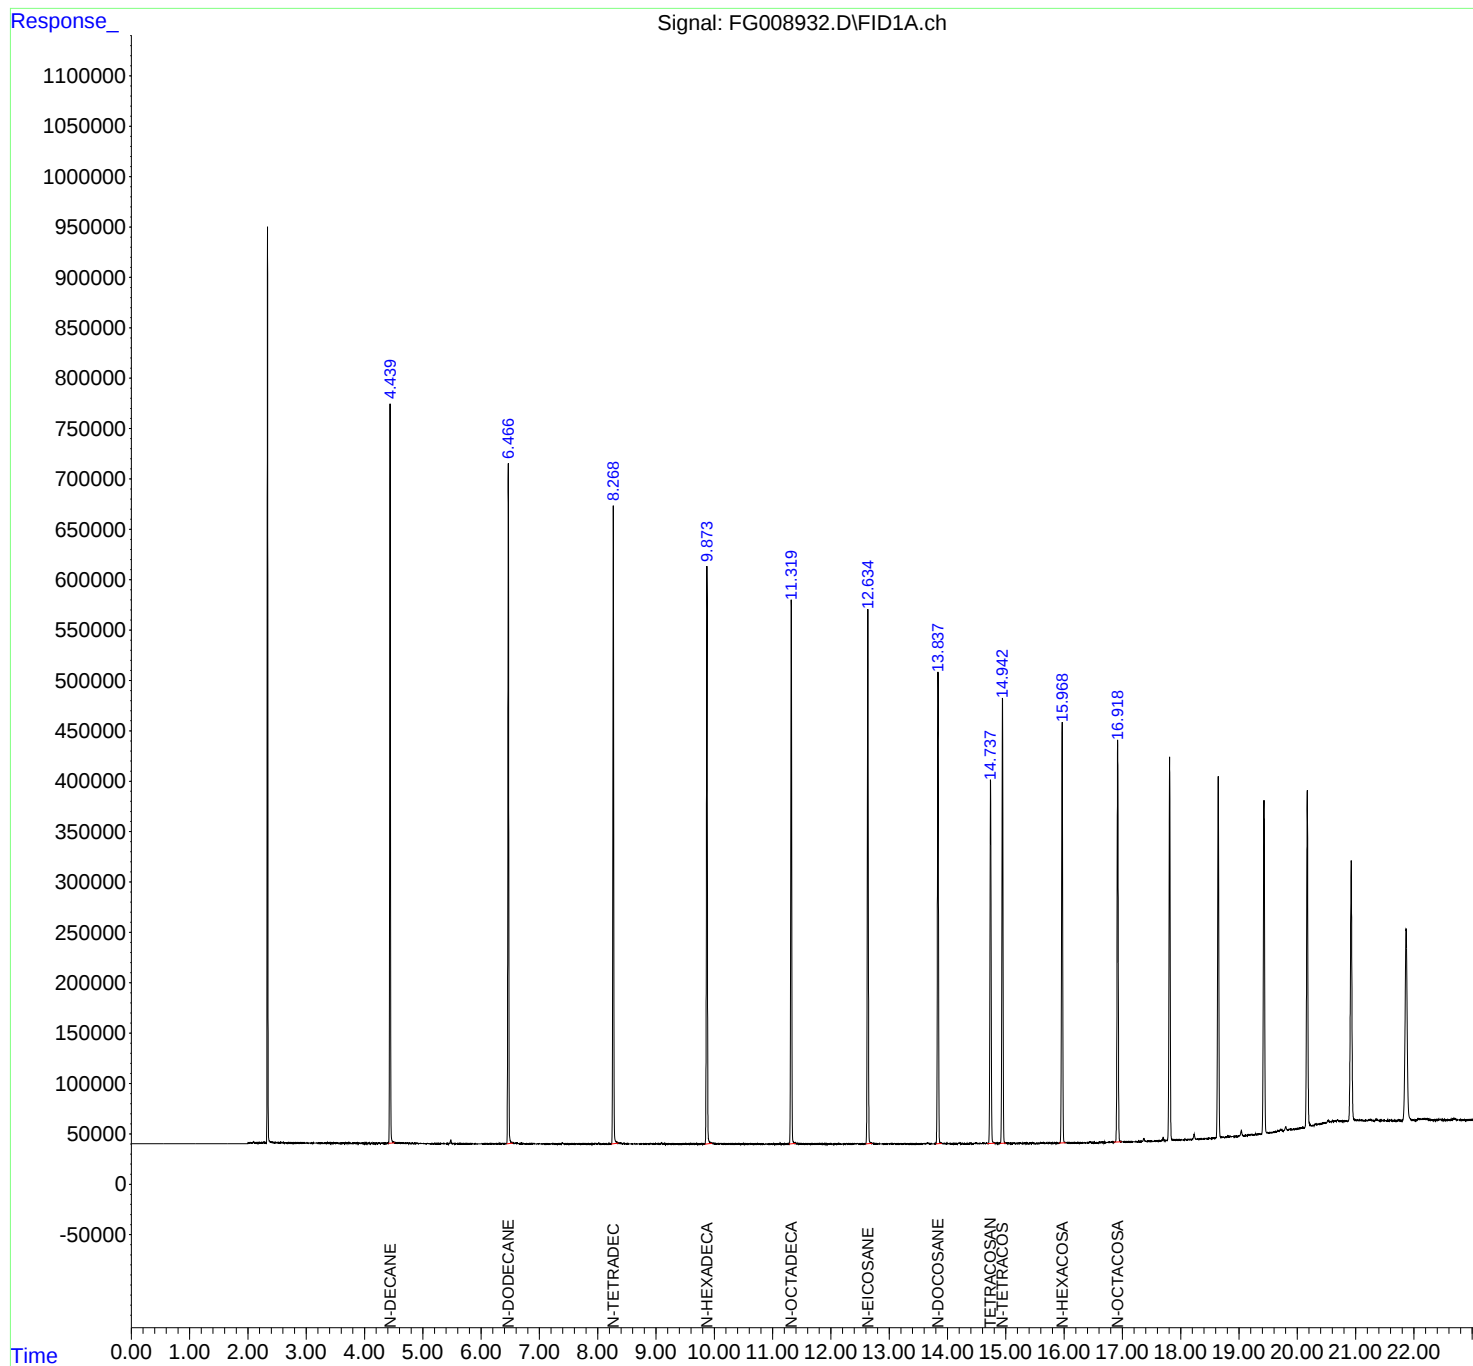


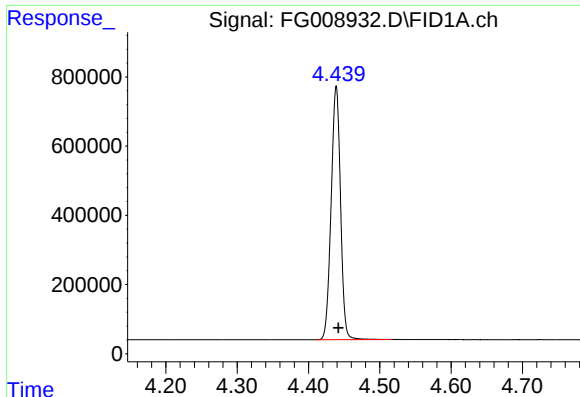

#2 N-DECANE


R.T.: 4.439 min
Delta R.T.: -0.003 min
Response: 6697136
Conc: 48.00 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

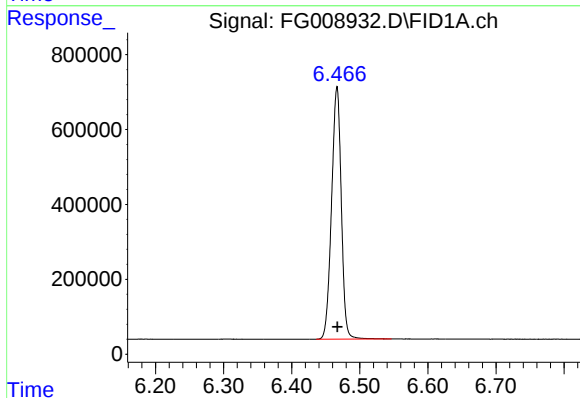


#3 N-DODECANE

R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 6677814
Conc: 47.36 ug/ml

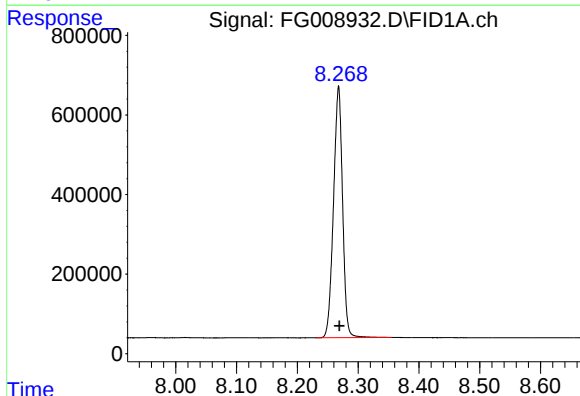


#4 N-TETRADECANE

R.T.: 8.268 min
Delta R.T.: -0.001 min
Response: 6553505
Conc: 46.49 ug/ml

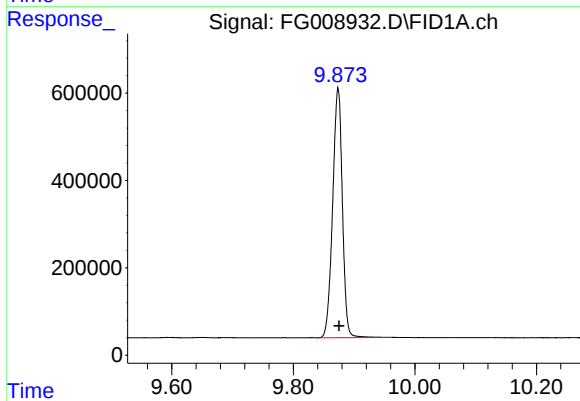

#5 N-HEXADECANE


R.T.: 9.874 min
Delta R.T.: -0.002 min
Response: 6351992
Conc: 45.36 ug/ml

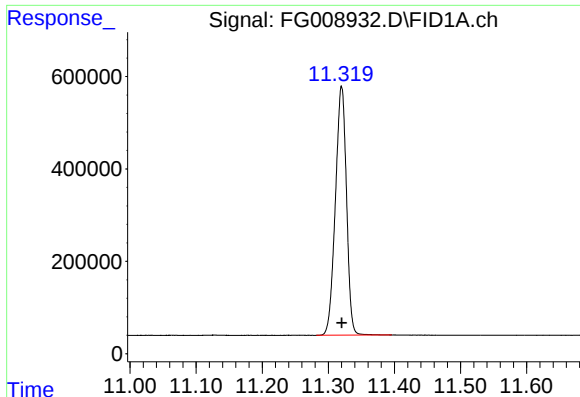

#6 N-OCTADECANE


R.T.: 11.320 min
Delta R.T.: 0.000 min
Response: 6285390
Conc: 44.48 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

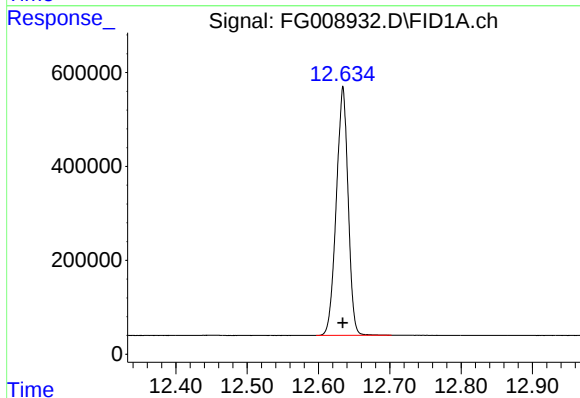


#7 N-EICOSANE

R.T.: 12.634 min
Delta R.T.: 0.000 min
Response: 6092834
Conc: 43.69 ug/ml

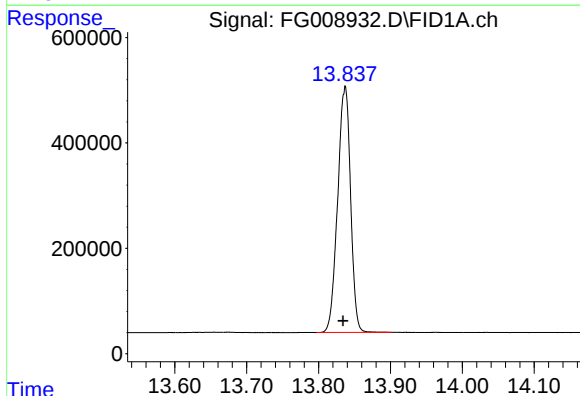


#8 N-DOCOSANE

R.T.: 13.837 min
Delta R.T.: 0.003 min
Response: 5821597
Conc: 43.16 ug/ml

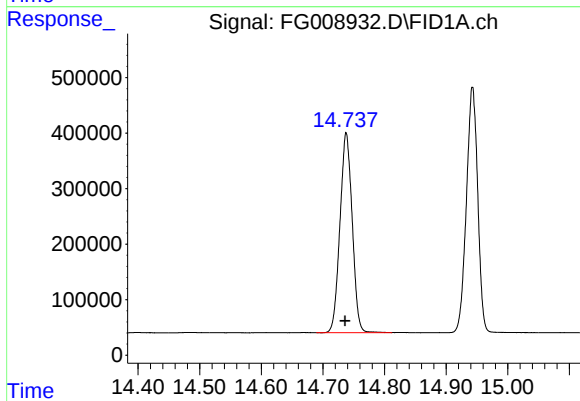

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.738 min
Delta R.T.: 0.002 min
Response: 4964917
Conc: 43.01 ug/ml

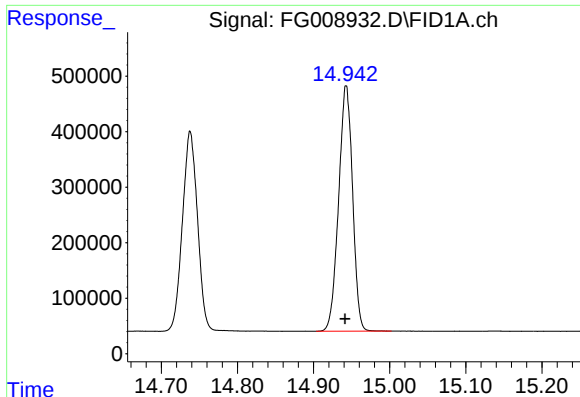

#10 N-TETRACOSANE


R.T.: 14.943 min
Delta R.T.: 0.001 min
Response: 5636069
Conc: 42.92 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

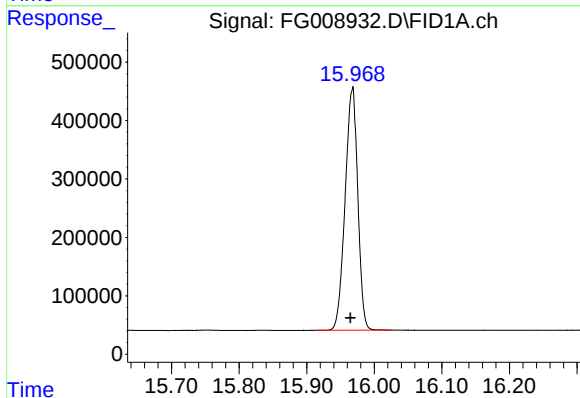

#11 N-HEXACOSANE

R.T.: 15.968 min
Delta R.T.: 0.003 min
Response: 5410723
Conc: 43.22 ug/ml

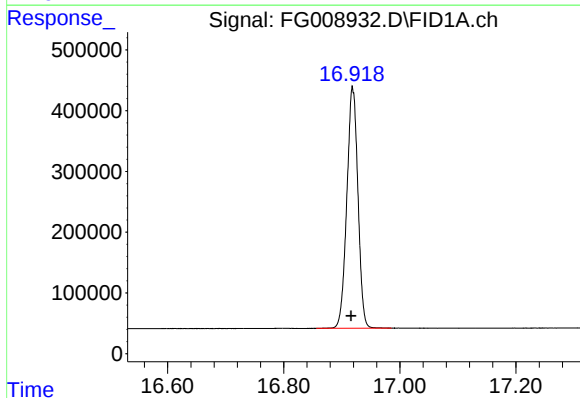

#12 N-OCTACOSANE

R.T.: 16.919 min
Delta R.T.: 0.002 min
Response: 5278496
Conc: 44.30 ug/ml