

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101822\
Data File : FG010929.D
Signal(s) : FID1A.ch
Acq On : 18 Oct 2022 16:14
Operator : YP\AJ
Sample : PB148410BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB148410BL

Integration File: Sample.e
Quant Time: Oct 19 04:46:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	2124188	17.509 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101822\
Data File : FG010929.D
Signal(s) : FID1A.ch
Acq On : 18 Oct 2022 16:14
Operator : YP\AJ
Sample : PB148410BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB148410BL

Integration File: Sample.e
Quant Time: Oct 19 04:46:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

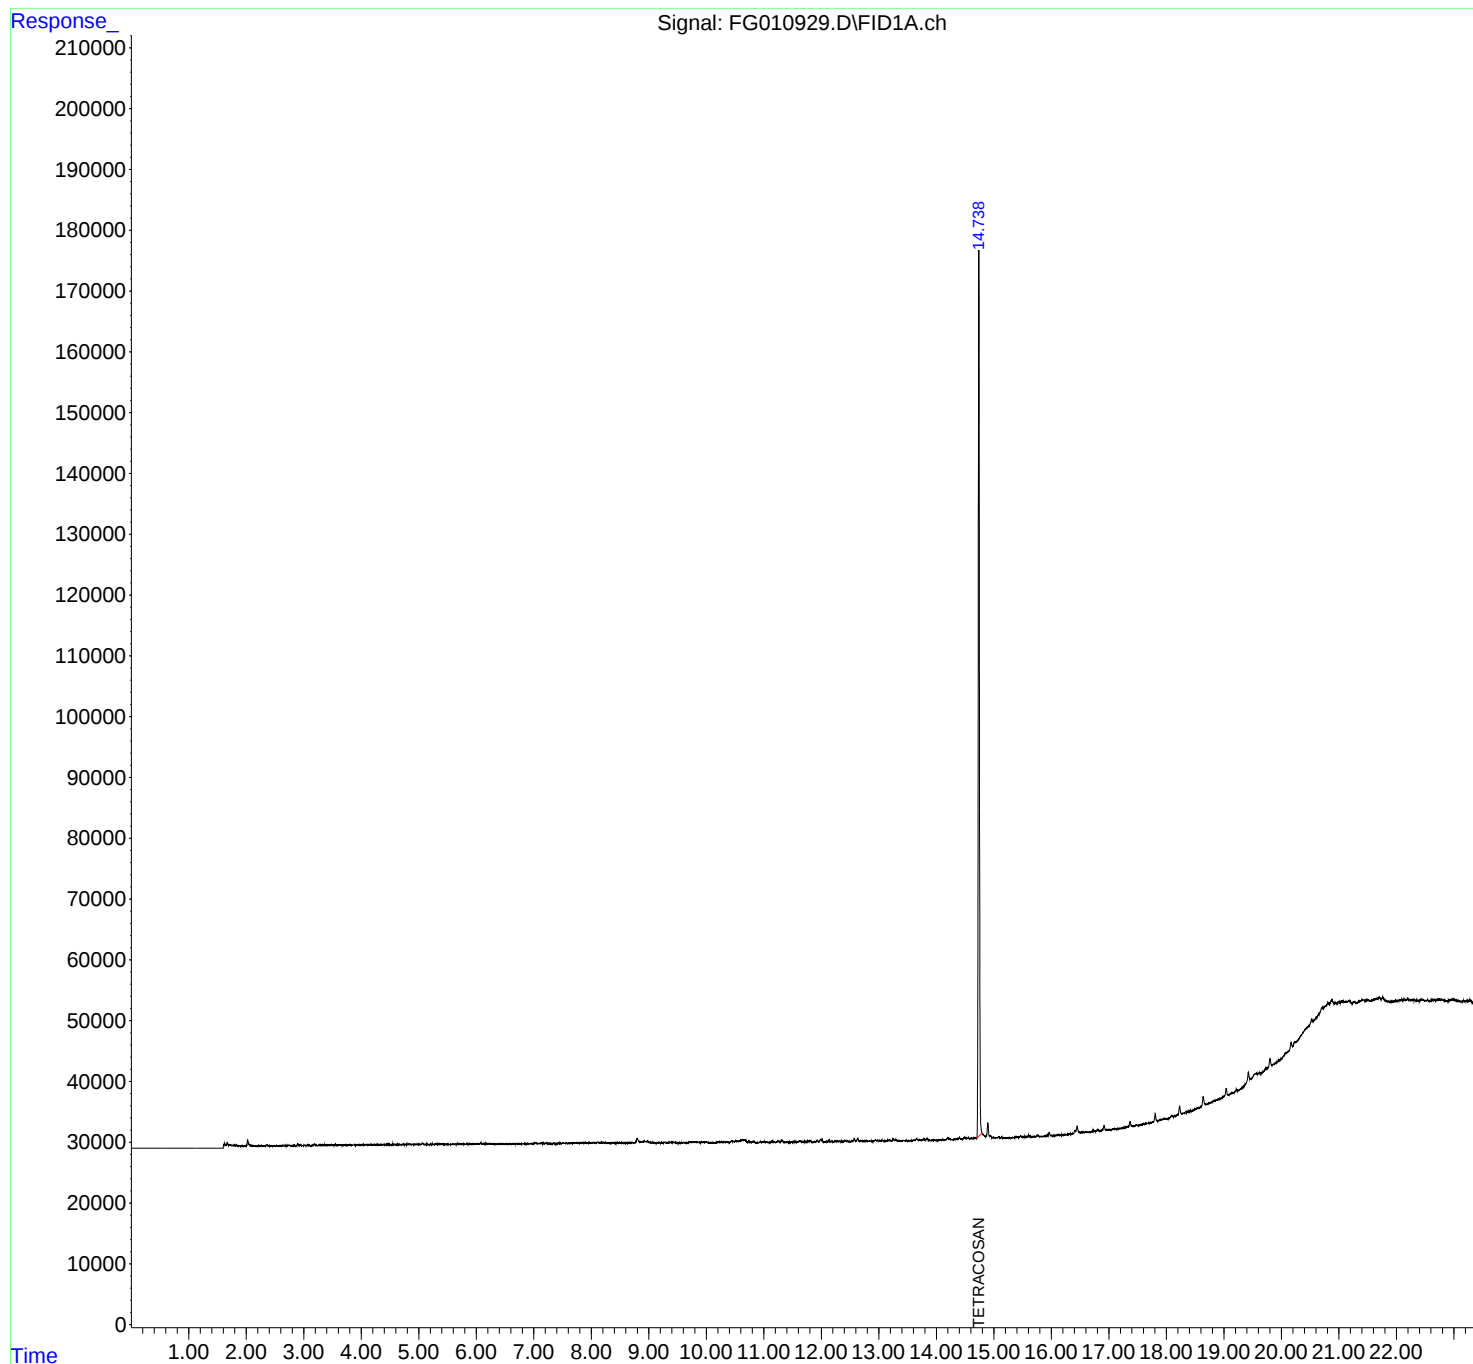

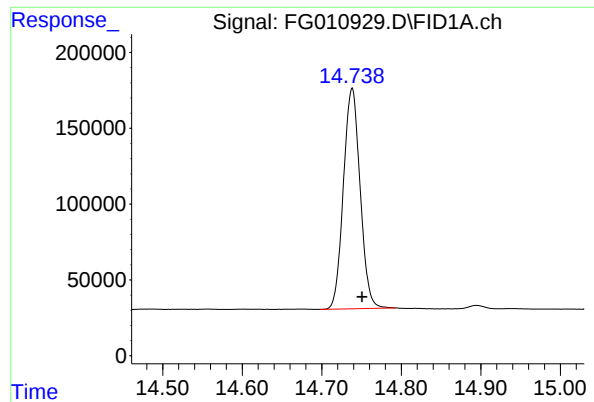

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: -0.013 min
Response: 2124188
Conc: 17.51 ug/ml

Instrument :
FID_G
ClientSampleId :
PB148410BL