

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101921\
Data File : FG008944.D
Signal(s) : FID1A.ch
Acq On : 19 Oct 2021 12:05
Operator : AJ\MA
Sample : PB139892BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 20 00:06:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	1999615	17.324 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.810	57385	0.506 ug/ml
14) N-DOTRIACONTANE	18.645	74289	0.700 ug/ml
15) N-TETRATRIACONTANE	19.429	52735	0.529 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101921\
Data File : FG008944.D
Signal(s) : FID1A.ch
Acq On : 19 Oct 2021 12:05
Operator : AJ\MA
Sample : PB139892BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 20 00:06:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

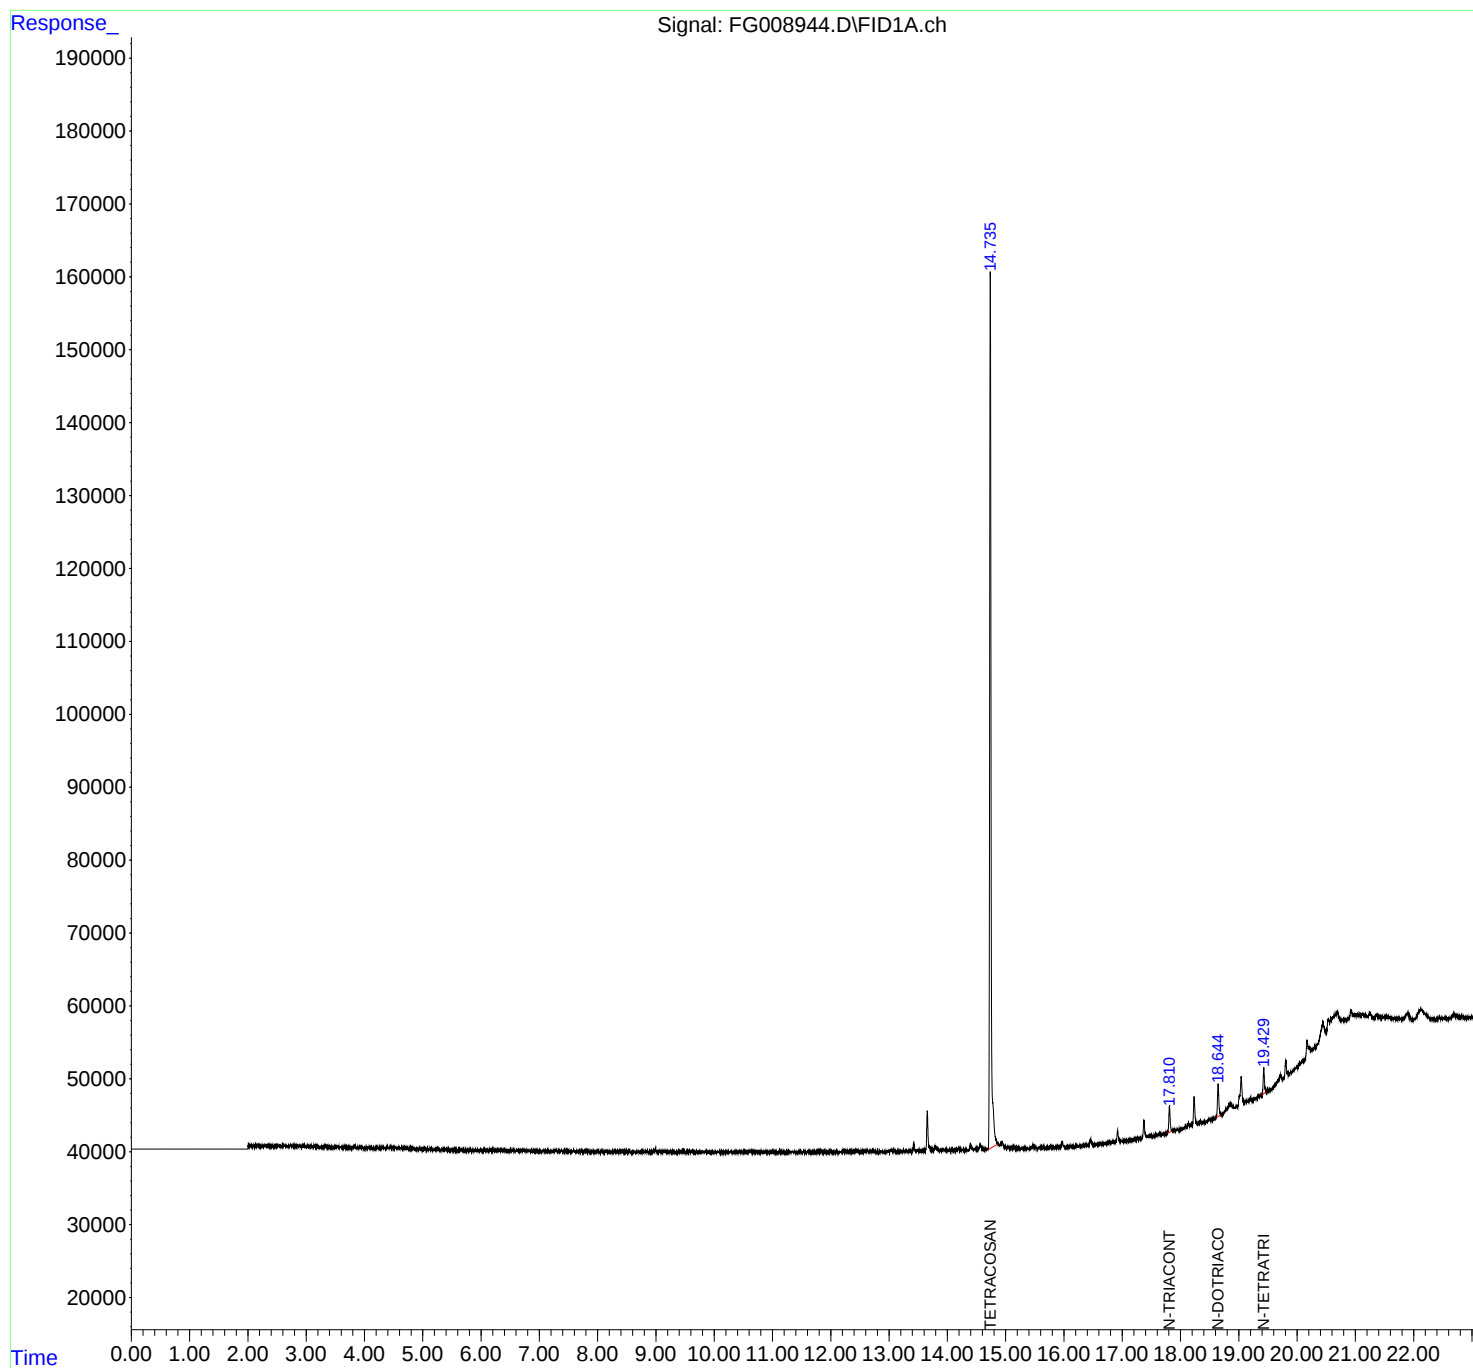


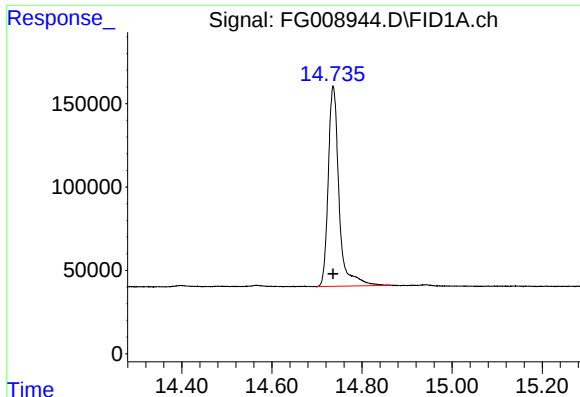

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.736 min
Delta R.T.: 0.000 min
Response: 1999615
Conc: 17.32 ug/ml

Instrument :
FID_G
ClientSampleId :

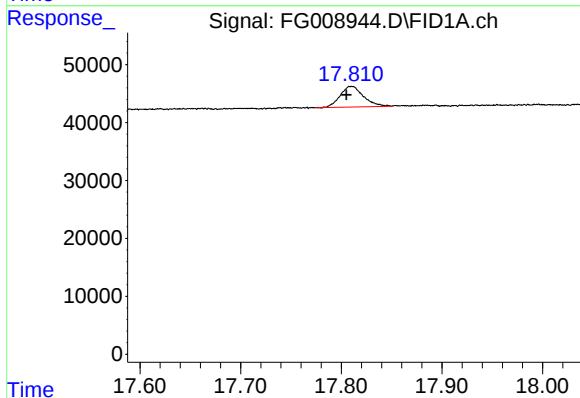


#13 N-TRIACONTANE

R.T.: 17.810 min
Delta R.T.: 0.005 min
Response: 57385
Conc: 0.51 ug/ml

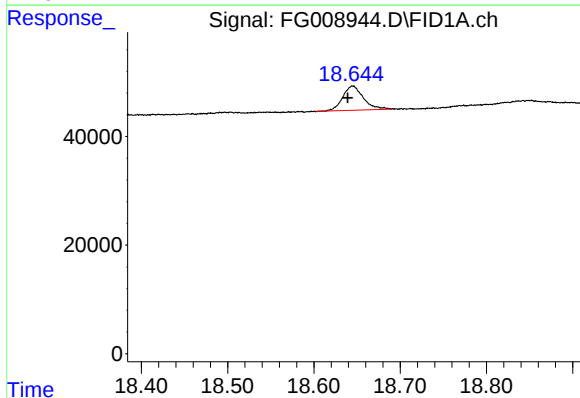

#14 N-DOTRIACONTANE

R.T.: 18.645 min
Delta R.T.: 0.005 min
Response: 74289
Conc: 0.70 ug/ml

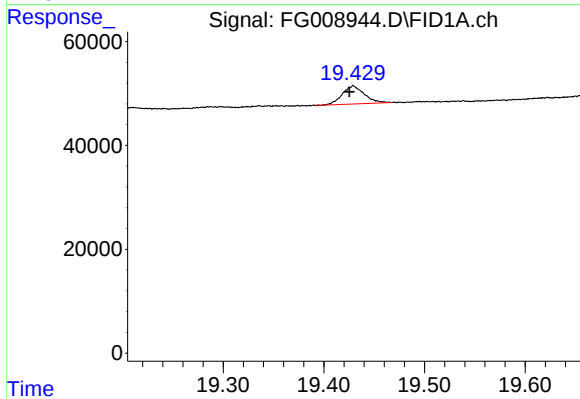

#15 N-TETRATRIACONTANE

R.T.: 19.429 min
Delta R.T.: 0.004 min
Response: 52735
Conc: 0.53 ug/ml