

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101921\
 Data File : FG008946.D
 Signal(s) : FID1A.ch
 Acq On : 19 Oct 2021 13:06
 Operator : AJ\MA
 Sample : PB139875BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 20 00:07:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
 Quant Title :
 QLast Update : Fri Oct 08 03:31:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	2053846	17.793 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.809	64346	0.567 ug/ml
14) N-DOTRIACONTANE	18.643	85083	0.802 ug/ml
15) N-TETRATRIACONTANE	19.427	68541	0.688 ug/ml
16) N-HEXATRIACONTANE	20.170	41697	0.451 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101921\
Data File : FG008946.D
Signal(s) : FID1A.ch
Acq On : 19 Oct 2021 13:06
Operator : AJ\MA
Sample : PB139875BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 20 00:07:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

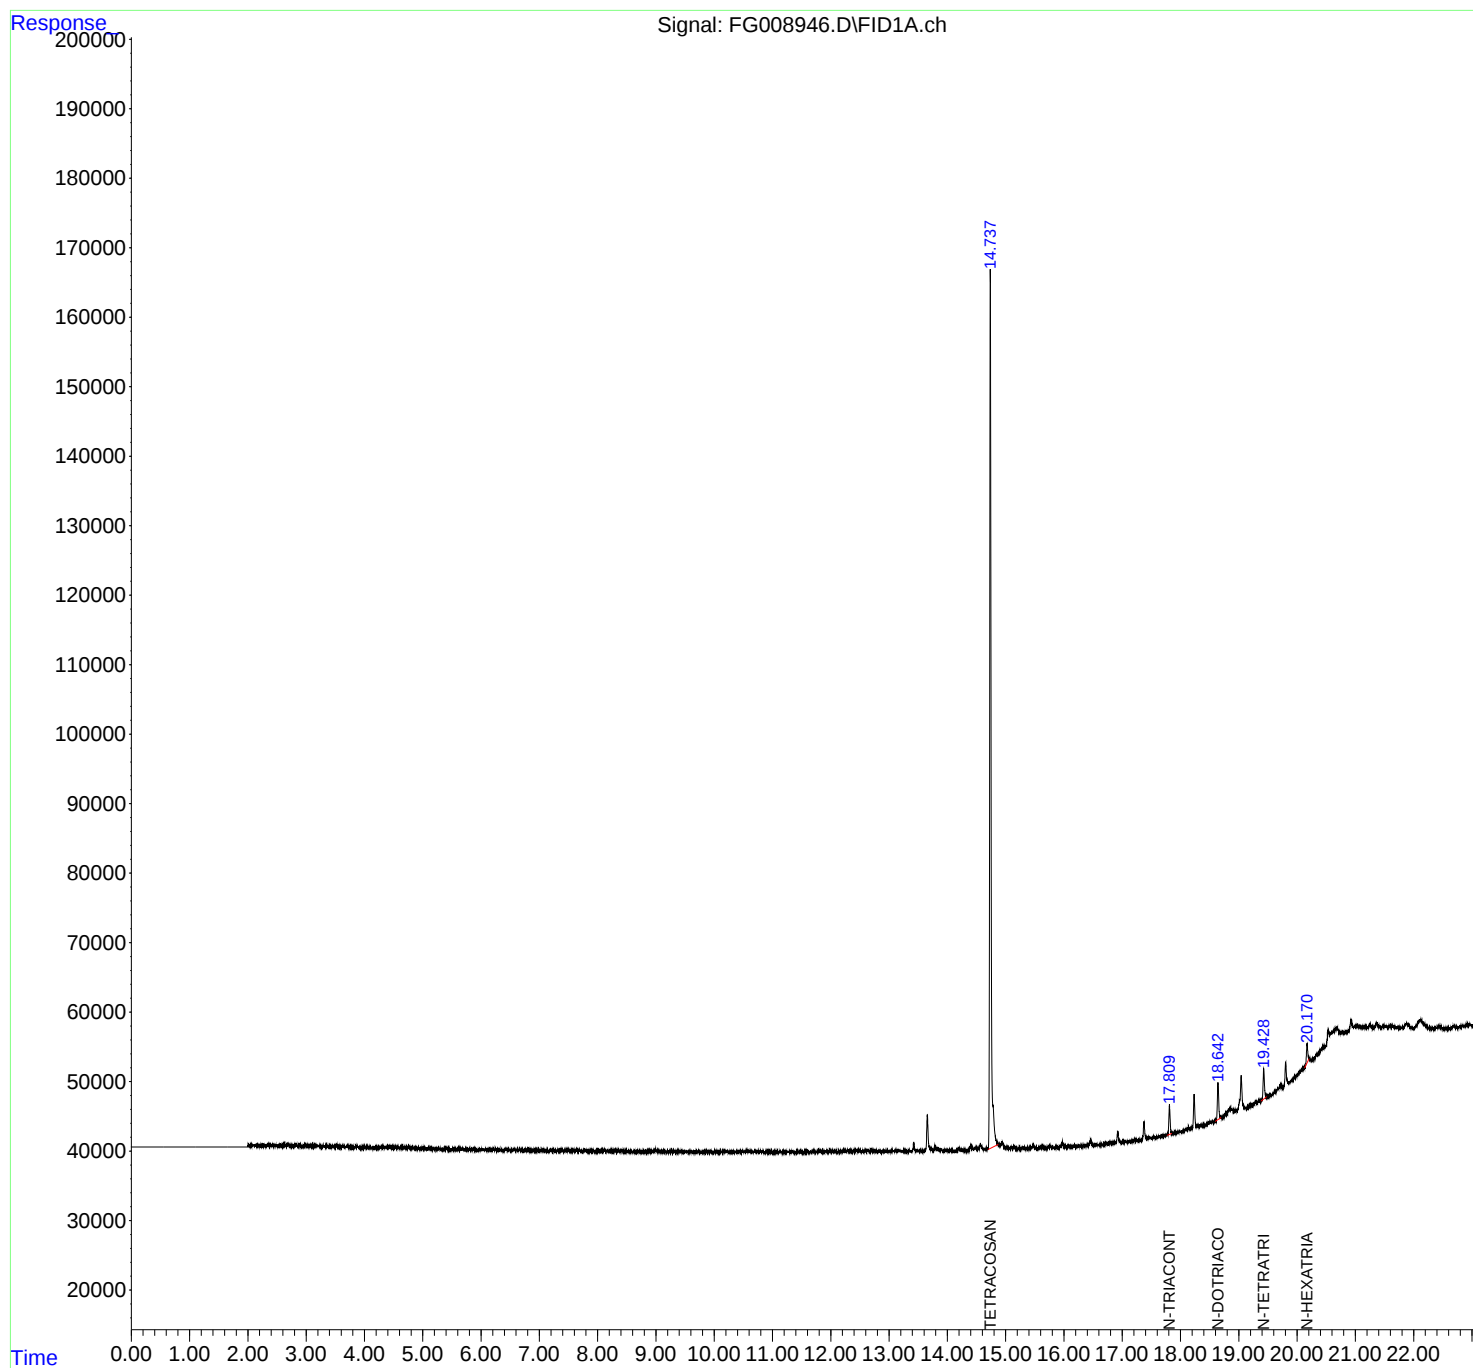


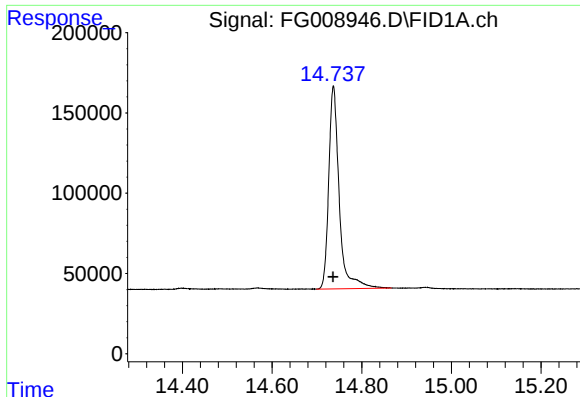

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.737 min
Delta R.T.: 0.001 min
Response: 2053846
Conc: 17.79 ug/ml

Instrument :
FID_G
ClientSampleId :

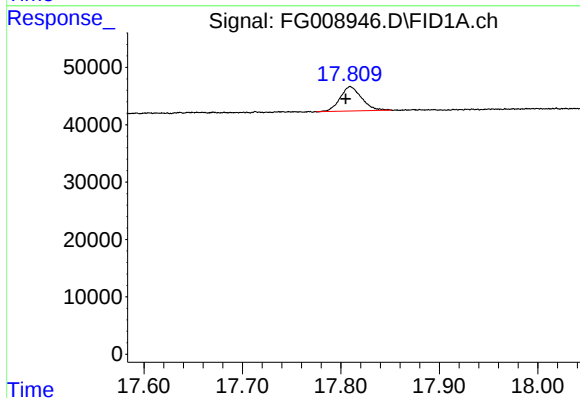


#13 N-TRIACONTANE

R.T.: 17.809 min
Delta R.T.: 0.004 min
Response: 64346
Conc: 0.57 ug/ml

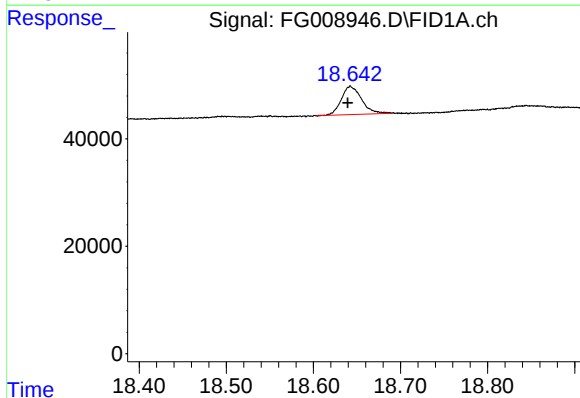


#14 N-DOTRIACONTANE

R.T.: 18.643 min
Delta R.T.: 0.003 min
Response: 85083
Conc: 0.80 ug/ml

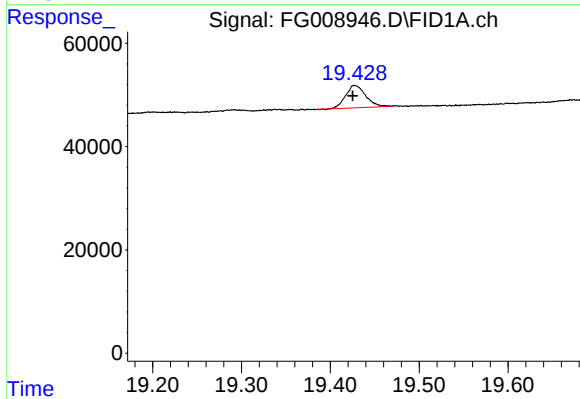

#15 N-TETRATRIACONTANE

R.T.: 19.427 min
Delta R.T.: 0.002 min
Response: 68541
Conc: 0.69 ug/ml

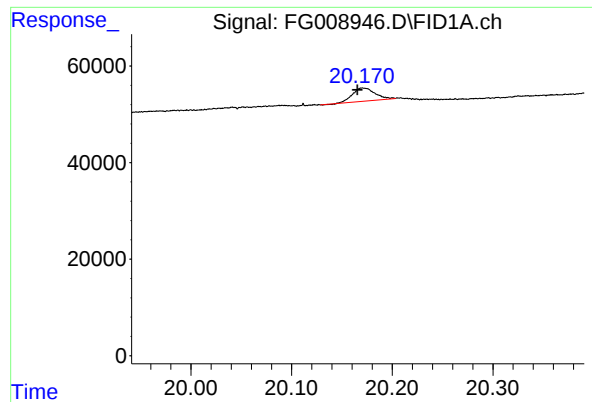

#16 N-HEXATRIACONTANE

R.T.: 20.170 min
Delta R.T.: 0.005 min
Response: 41697
Conc: 0.45 ug/ml

Instrument :
FID_G
ClientSampleId :