

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101921\
Data File : FG008943.D
Signal(s) : FID1A.ch
Acq On : 19 Oct 2021 11:35
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 20 00:06:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.464	3776521	26.783 ug/ml
12) N-OCTACOSANE	16.919	3766512	31.608 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG101921\
Data File : FG008943.D
Signal(s) : FID1A.ch
Acq On : 19 Oct 2021 11:35
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 20 00:06:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100721.M
Quant Title :
QLast Update : Fri Oct 08 03:31:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

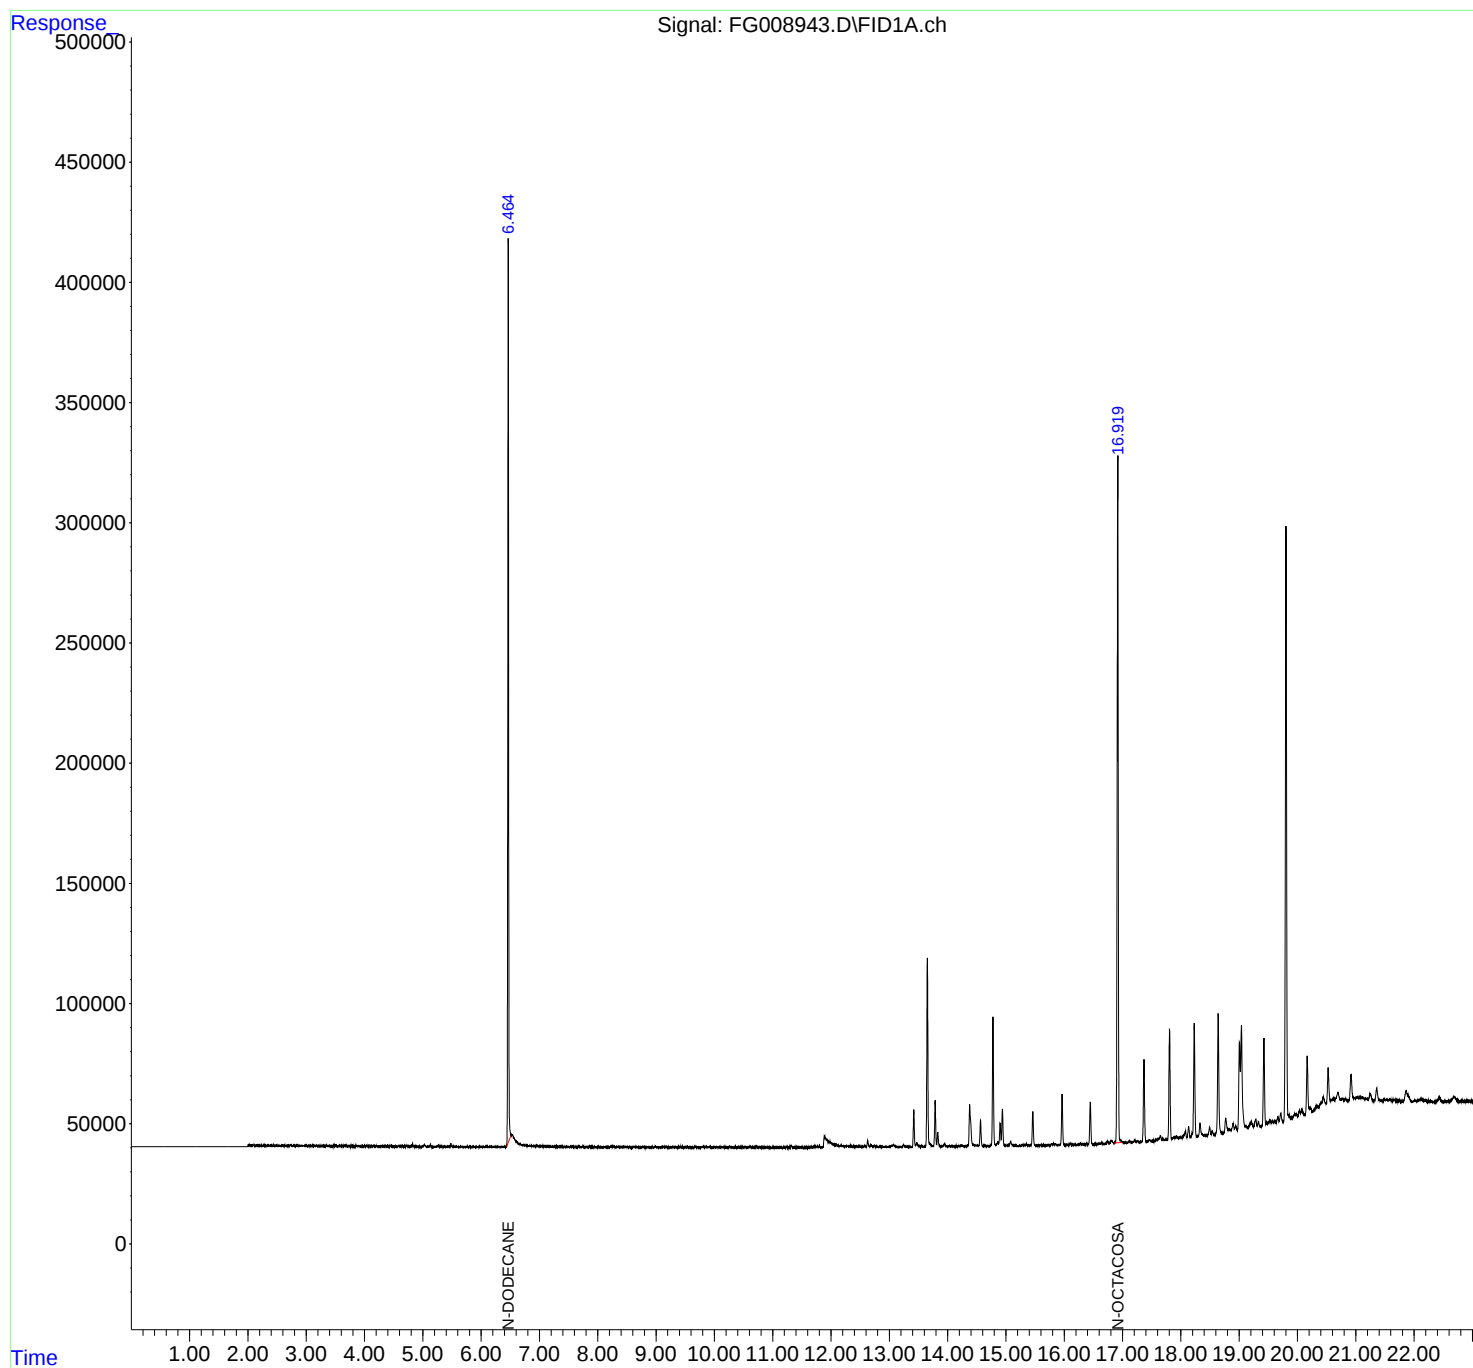


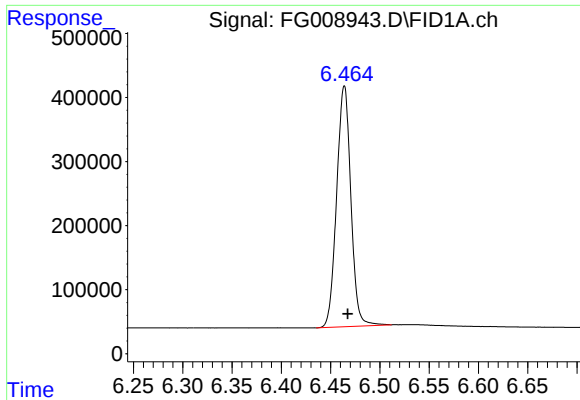

#3 N-DODECANE


R.T.: 6.464 min
Delta R.T.: -0.003 min
Response: 3776521
Conc: 26.78 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

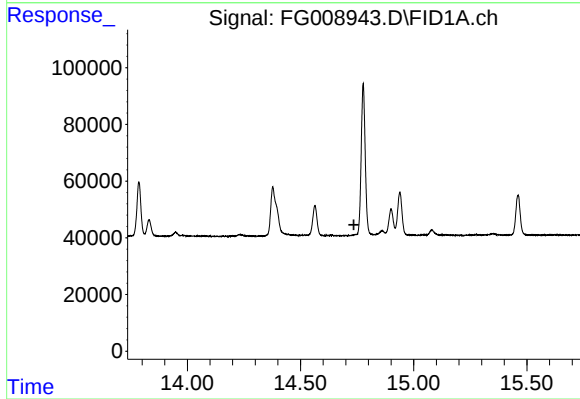

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.736 min
Response: 0
Conc: N.D.

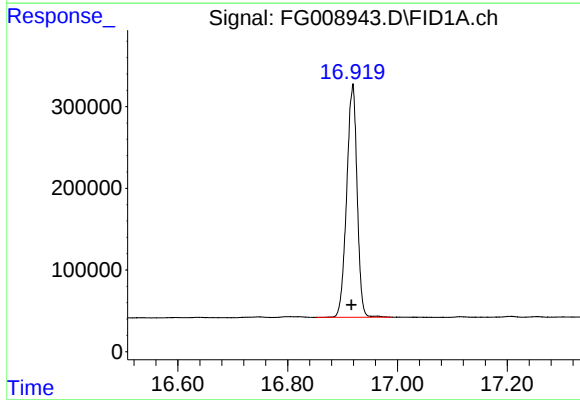

#12 N-OCTACOSANE

R.T.: 16.919 min
Delta R.T.: 0.003 min
Response: 3766512
Conc: 31.61 ug/ml