

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG102422\  
Data File : FG010971.D  
Signal(s) : FID1A.ch  
Acq On : 24 Oct 2022 10:18  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 25 06:05:16 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG092822.M  
Quant Title :  
QLast Update : Thu Sep 29 02:21:49 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                 | R.T.    | Response | Conc Units  |
|-----------------------------|-----------------|---------|----------|-------------|
| -----                       |                 |         |          |             |
| System Monitoring Compounds |                 |         |          |             |
| Target Compounds            |                 |         |          |             |
| 10)                         | N-TETRACOSANE   | 14.893f | 988043   | 7.172 ug/ml |
| 14)                         | N-DOTRIACONTANE | 18.639  | 389484   | 3.065 ug/ml |
| -----                       |                 |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG102422\  
Data File : FG010971.D  
Signal(s) : FID1A.ch  
Acq On : 24 Oct 2022 10:18  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 25 06:05:16 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG092822.M  
Quant Title :  
QLast Update : Thu Sep 29 02:21:49 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

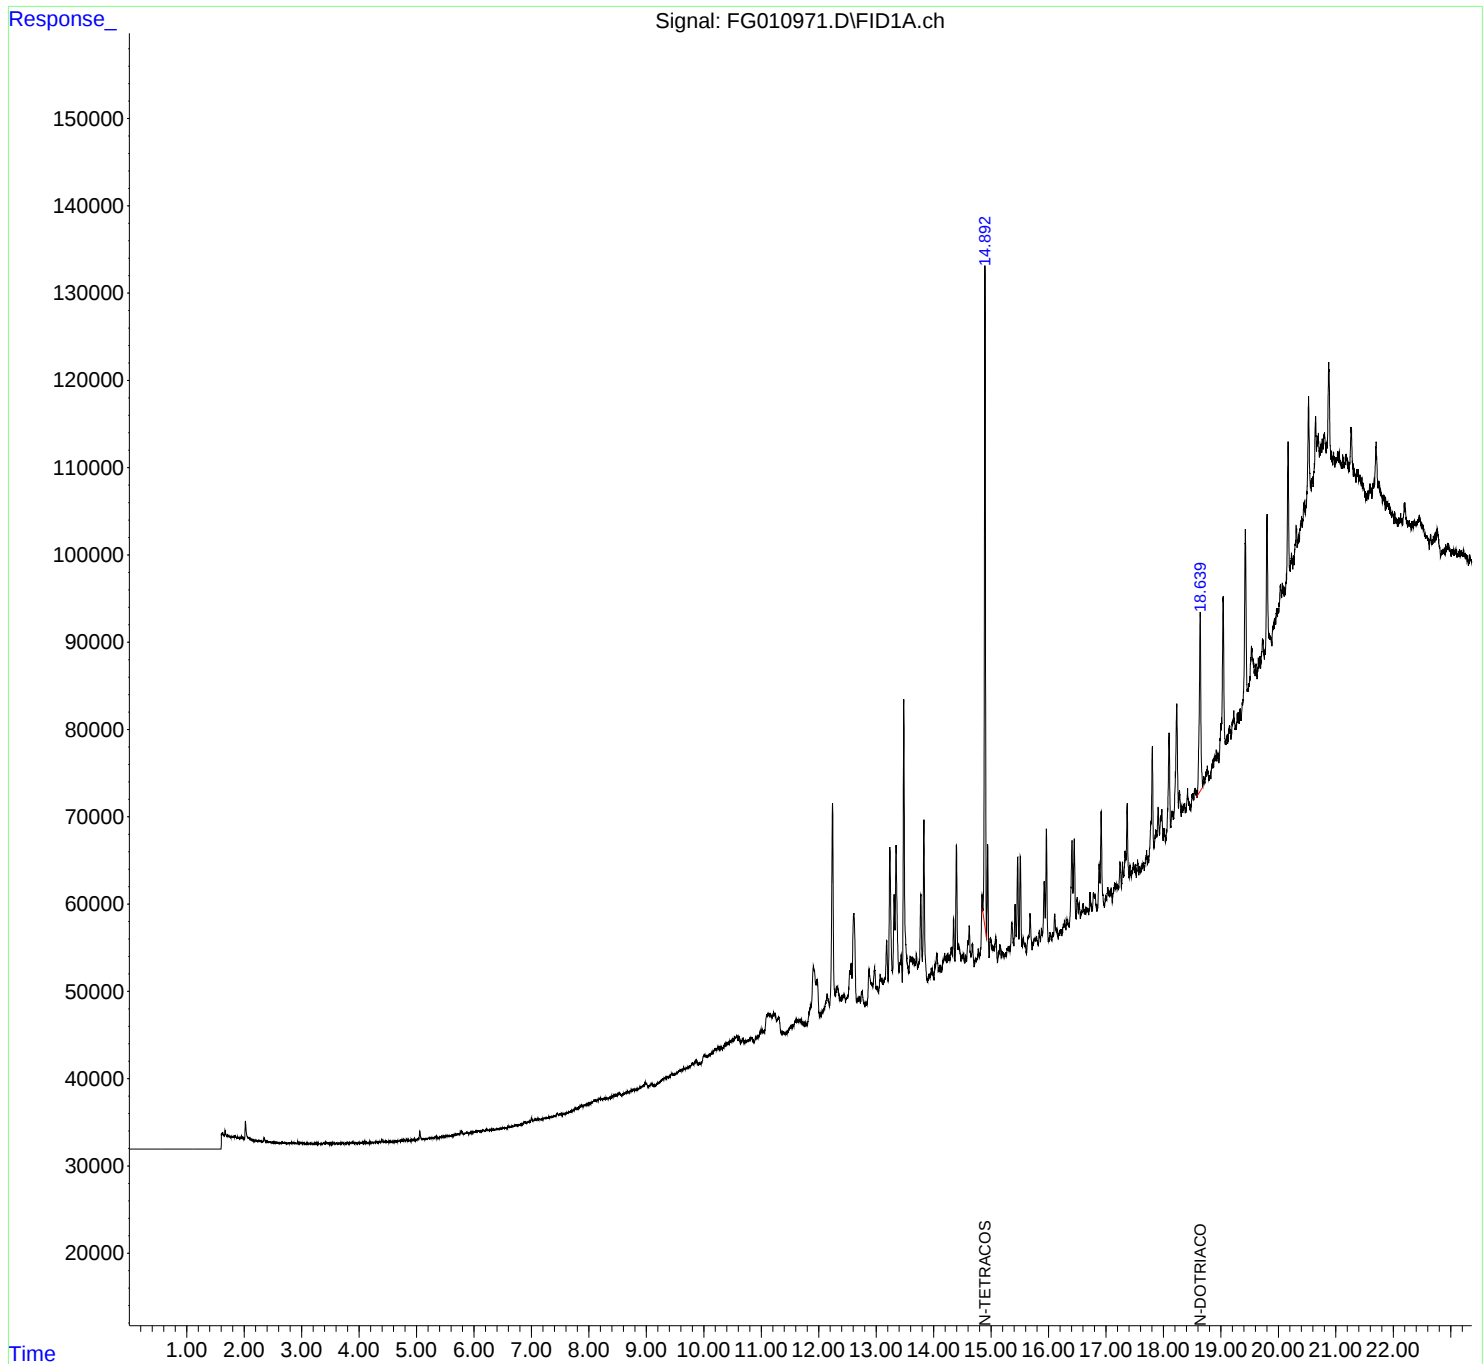


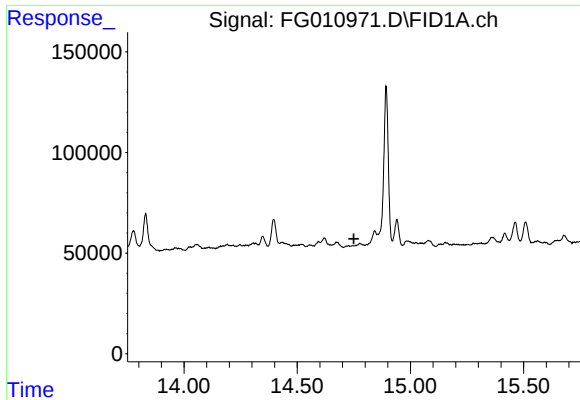

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min  
Exp R.T.: 14.751 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_G  
ClientSampleId :

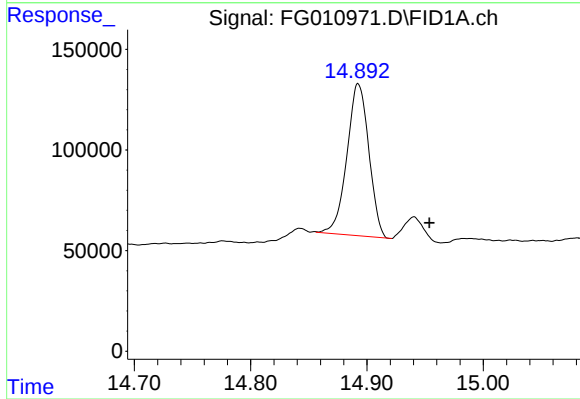

#10 N-TETRACOSANE

R.T.: 14.893 min  
Delta R.T.: -0.061 min  
Response: 988043  
Conc: 7.17 ug/ml

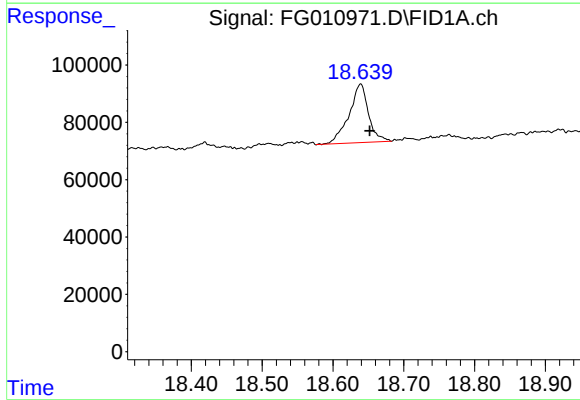

#14 N-DOTRIACONTANE

R.T.: 18.639 min  
Delta R.T.: -0.013 min  
Response: 389484  
Conc: 3.07 ug/ml