

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010994.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 23:11
Operator : YP\AJ
Sample : N5235-05 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 25 06:07:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.706f	188207	1.481 ug/ml
16)	N-HEXATRIACONTANE	20.124f	138891	1.153 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010994.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 23:11
Operator : YP\AJ
Sample : N5235-05 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 25 06:07:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

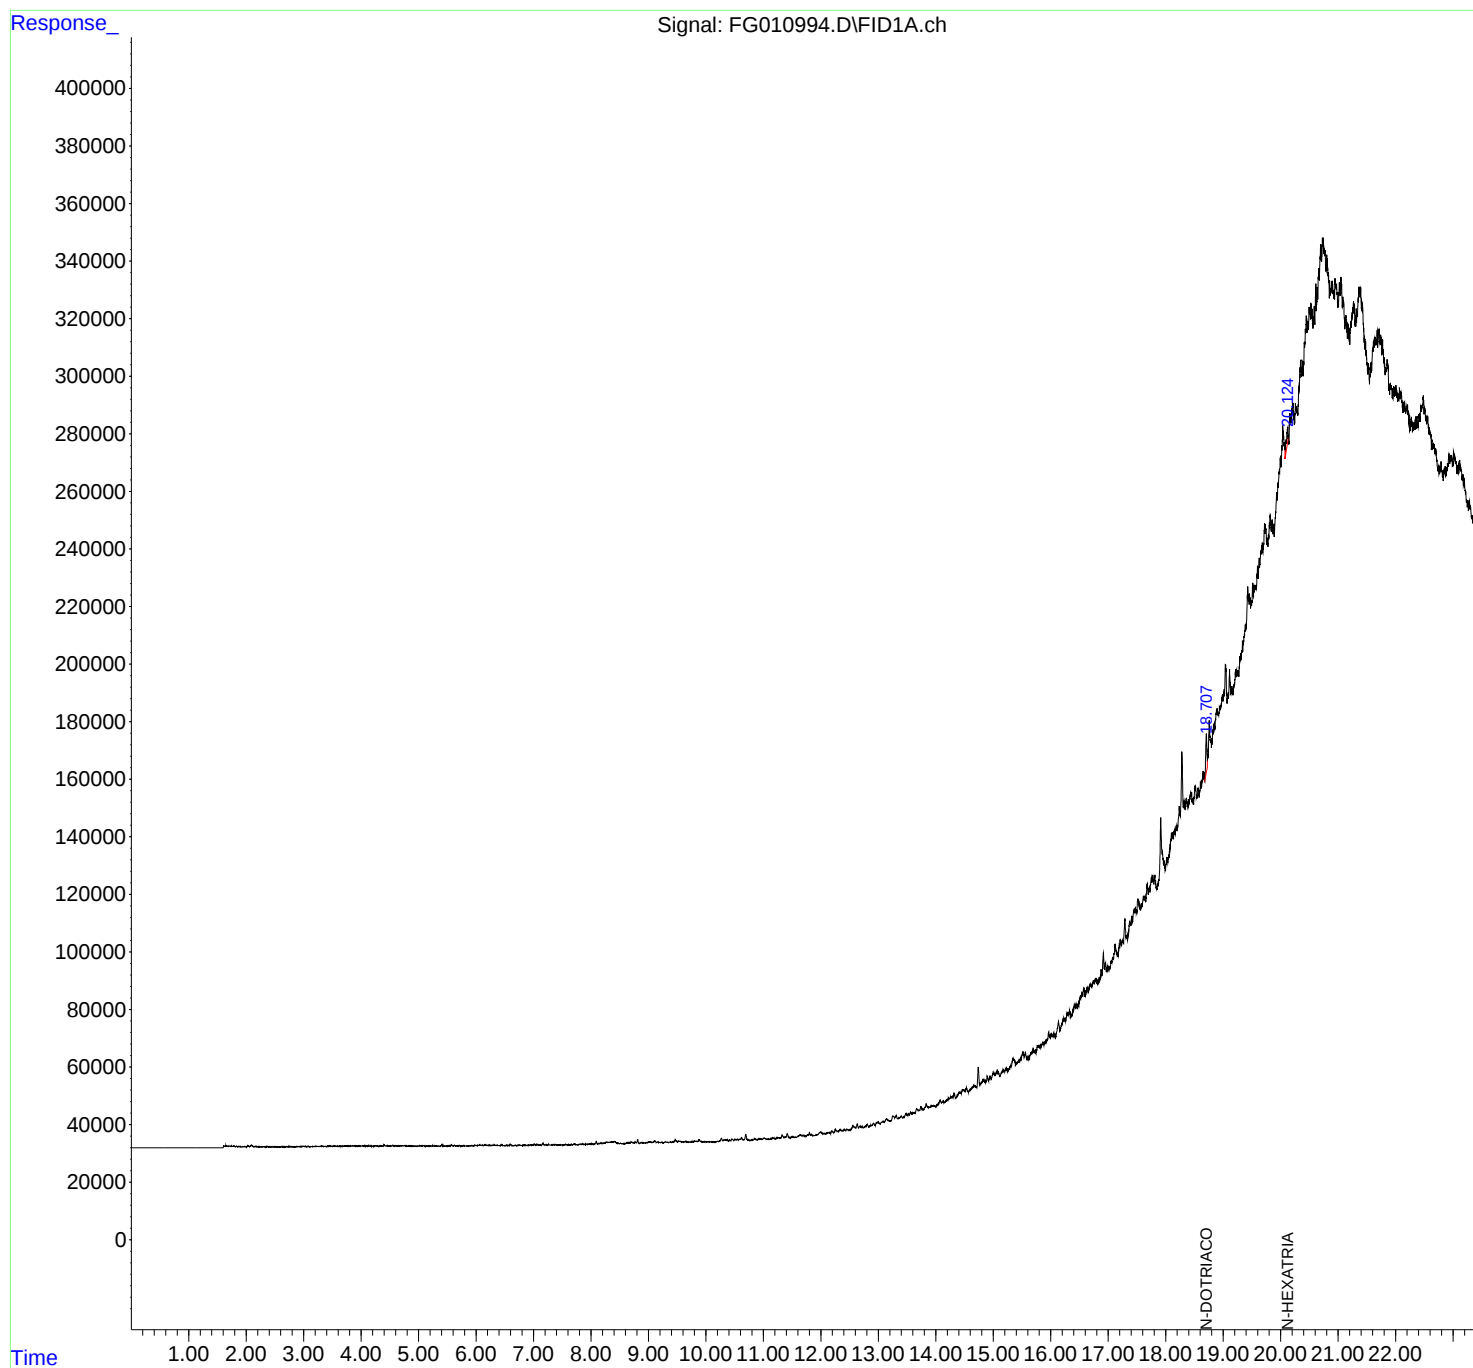


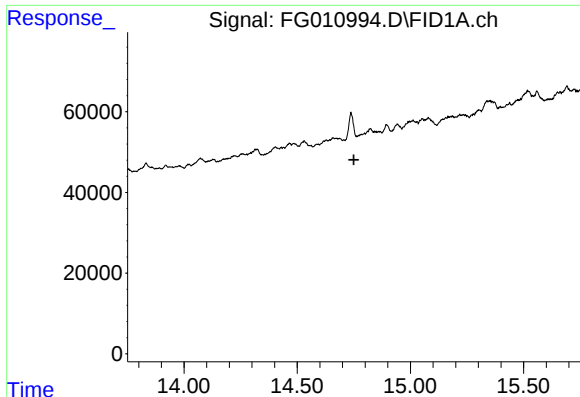

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.751 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

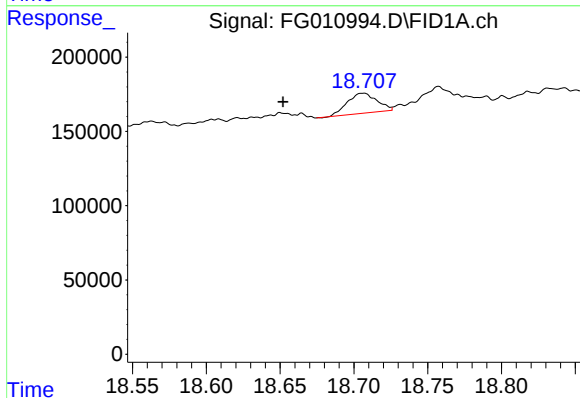

#14 N-DOTRIACONTANE

R.T.: 18.706 min
Delta R.T.: 0.054 min
Response: 188207
Conc: 1.48 ug/ml

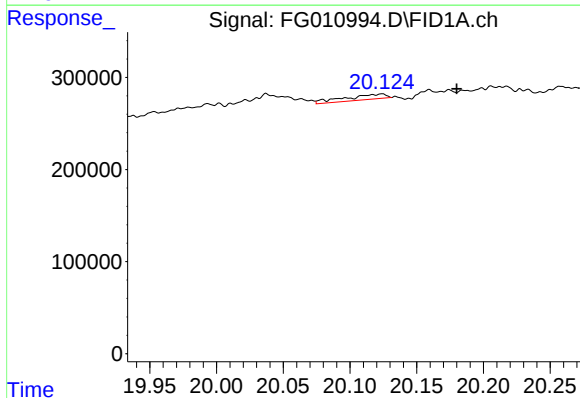

#16 N-HEXATRIACONTANE

R.T.: 20.124 min
Delta R.T.: -0.056 min
Response: 138891
Conc: 1.15 ug/ml