

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010976.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 12:49
Operator : YP\AJ
Sample : N5217-20 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-E1-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022

Integration File: autoint1.e
Quant Time: Oct 25 06:05:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	295684	2.437 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010976.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 12:49
Operator : YP\AJ
Sample : N5217-20 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
SB-E1-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022

Integration File: autoint1.e
Quant Time: Oct 25 06:05:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

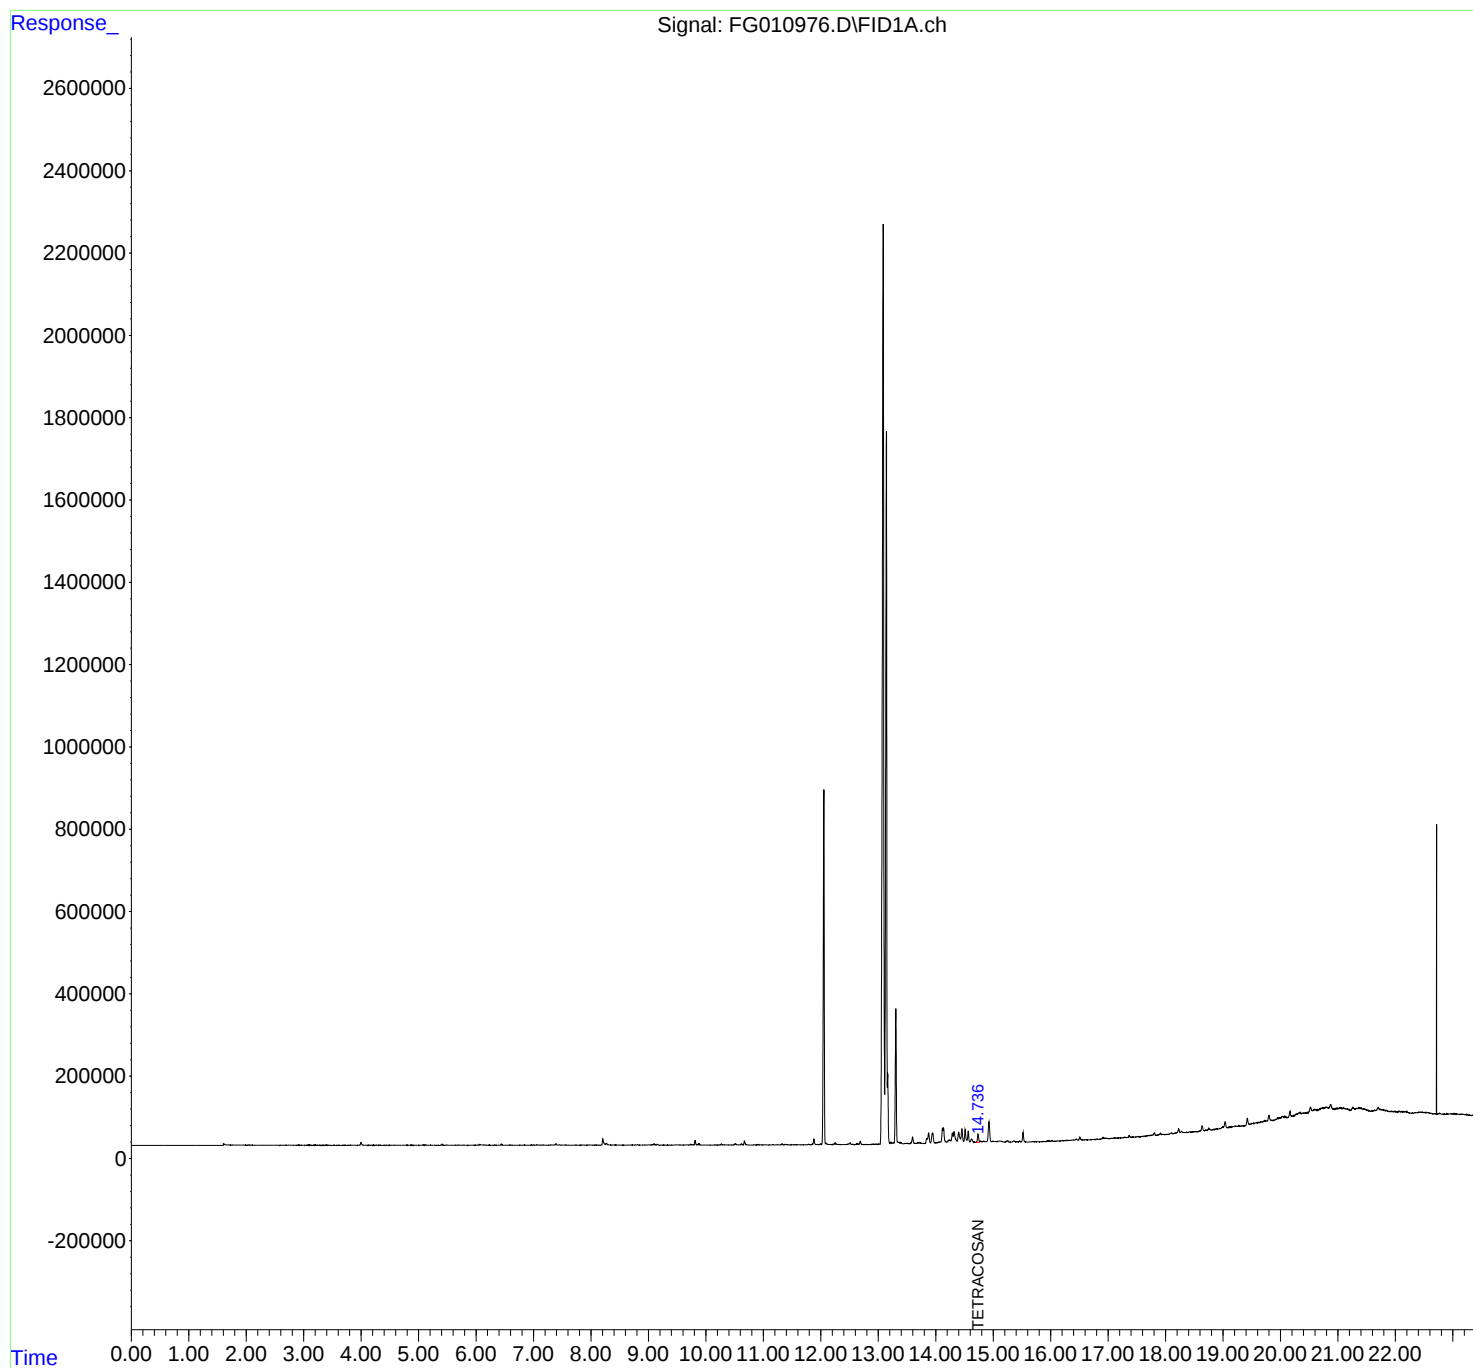

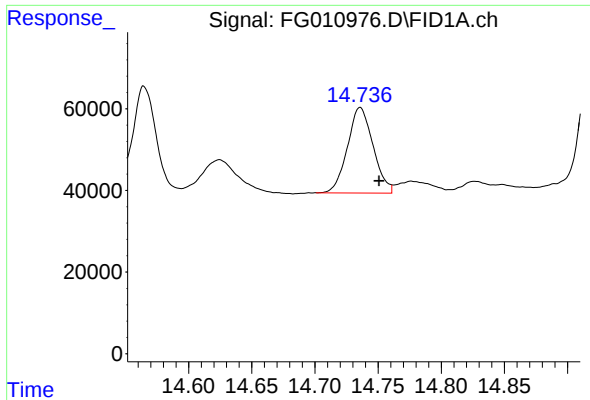

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.015 min
Response: 295684
Conc: 2.44 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-E1-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022