

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
 Data File : FG010978.D
 Signal(s) : FID1A.ch
 Acq On : 24 Oct 2022 14:18
 Operator : YP\AJ
 Sample : PB148516BS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB148516BS

Integration File: autoint1.e
 Quant Time: Oct 25 06:06:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
 Quant Title :
 QLast Update : Thu Sep 29 02:21:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	2356088	19.420 ug/ml
Target Compounds			
2) N-DECANE	4.258	2667467	20.497 ug/ml
3) N-DODECANE	6.441	2743980	20.691 ug/ml
4) N-TETRADECANE	8.272	2782638	20.752 ug/ml
5) N-HEXADECANE	9.881	2914579	21.020 ug/ml
6) N-OCTADECANE	11.325	3028974	21.492 ug/ml
7) N-EICOSANE	12.636	2981957	21.087 ug/ml
8) N-DOCOSANE	13.836	2941200	21.247 ug/ml
10) N-TETRACOSANE	14.941	2879341	20.899 ug/ml
11) N-HEXACOSANE	15.964	2818352	20.890 ug/ml
12) N-OCTACOSANE	16.916	2743524	20.921 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010978.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 14:18
Operator : YP\AJ
Sample : PB148516BS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB148516BS

Integration File: autoint1.e
Quant Time: Oct 25 06:06:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

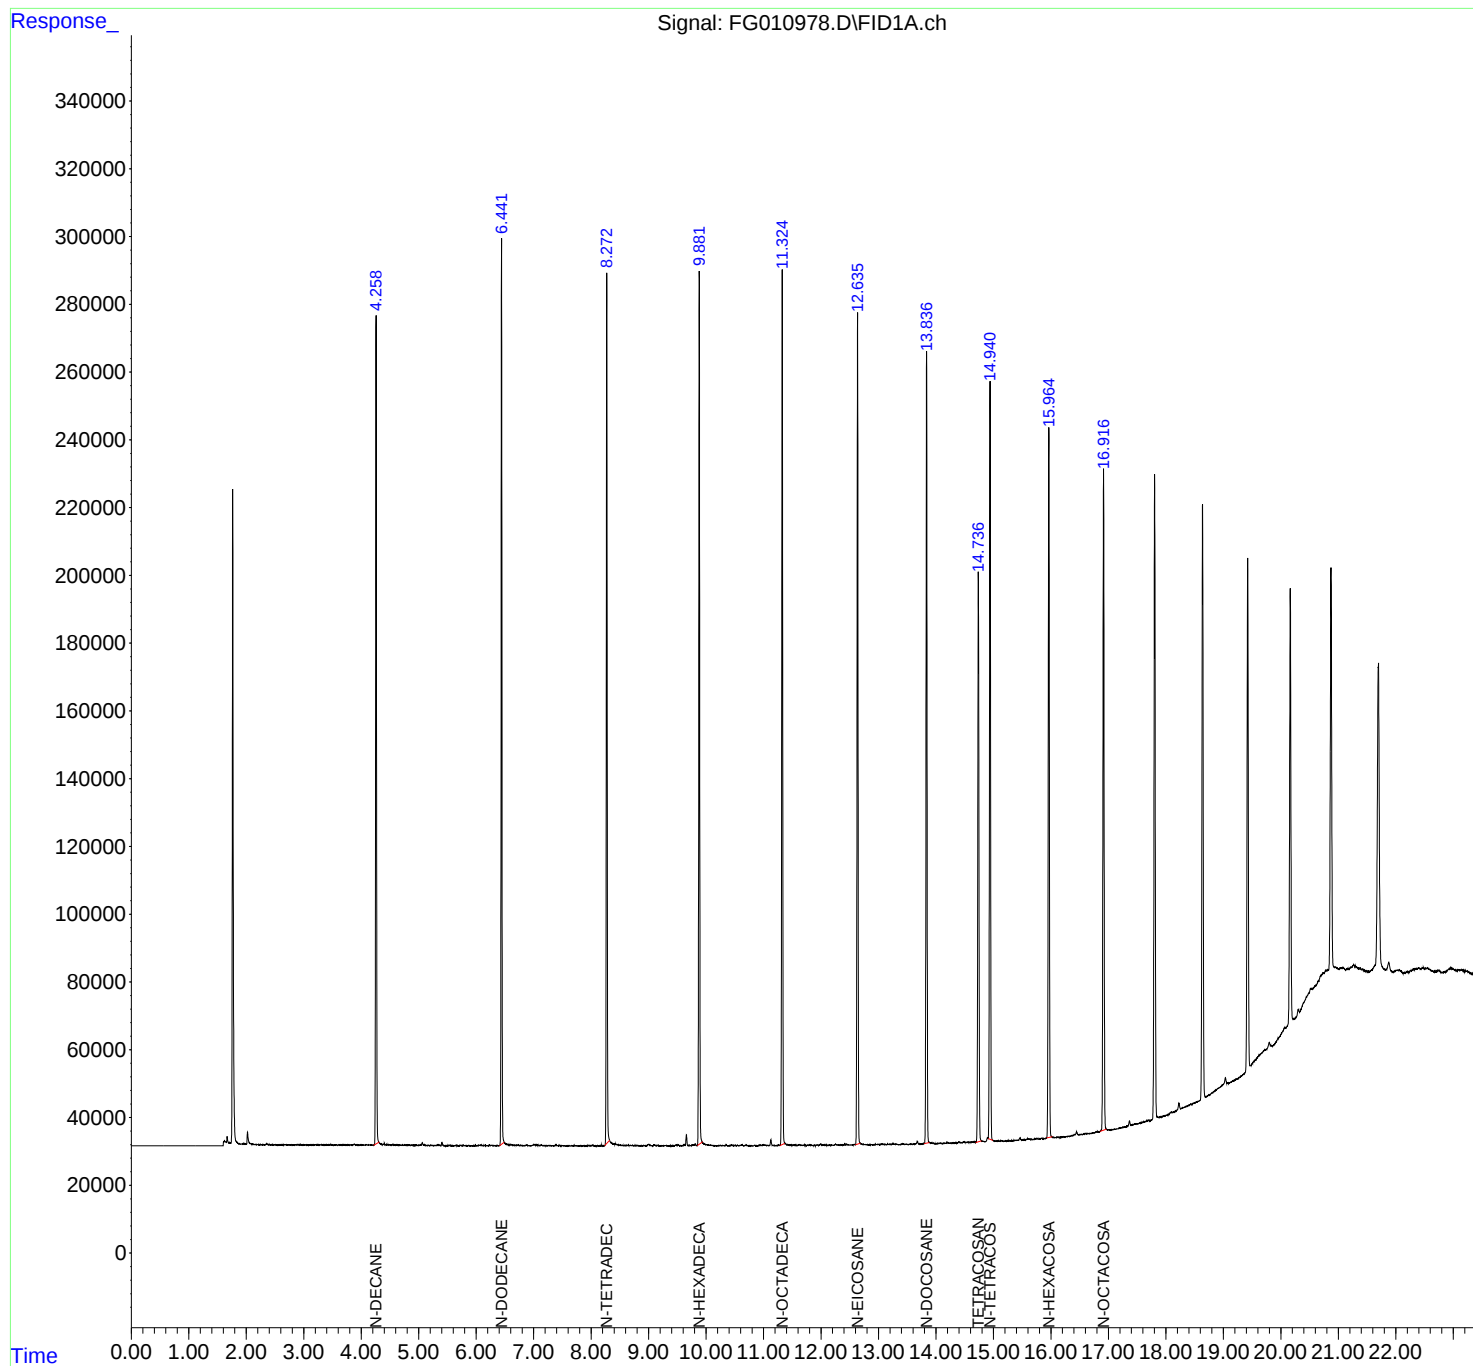


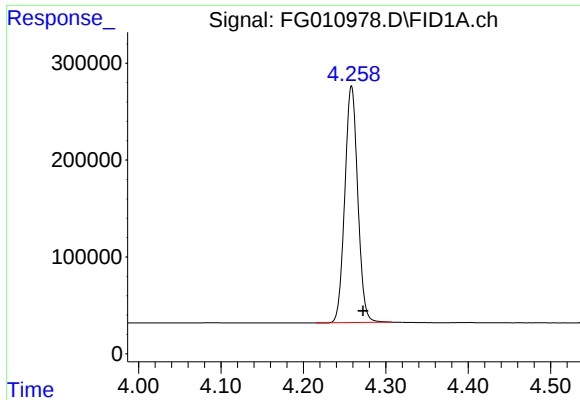

#2 N-DECANE


R.T.: 4.258 min
Delta R.T.: -0.014 min
Response: 2667467
Conc: 20.50 ug/ml

Instrument :
FID_G
ClientSampleId :
PB148516BS

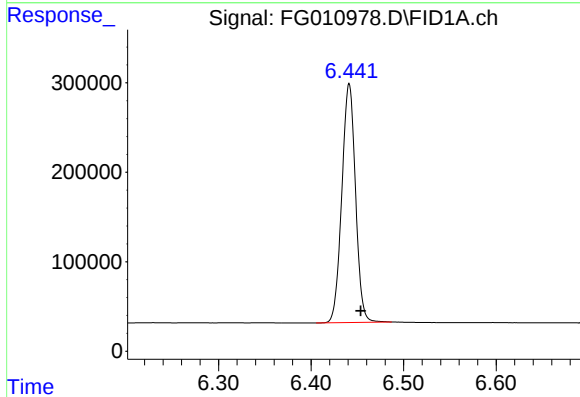


#3 N-DODECANE

R.T.: 6.441 min
Delta R.T.: -0.012 min
Response: 2743980
Conc: 20.69 ug/ml

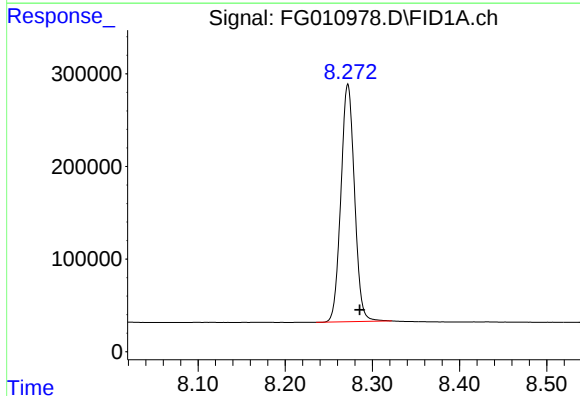


#4 N-TETRADECANE

R.T.: 8.272 min
Delta R.T.: -0.013 min
Response: 2782638
Conc: 20.75 ug/ml

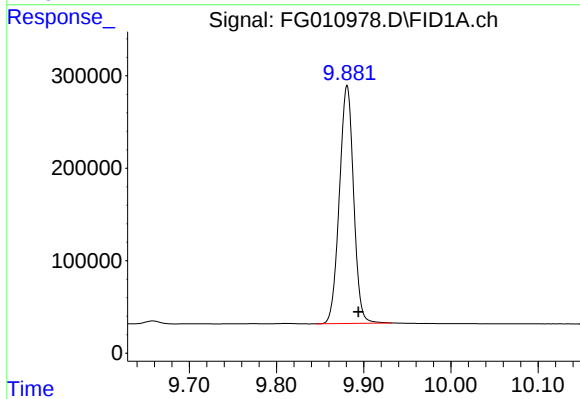

#5 N-HEXADECANE


R.T.: 9.881 min
Delta R.T.: -0.013 min
Response: 2914579
Conc: 21.02 ug/ml

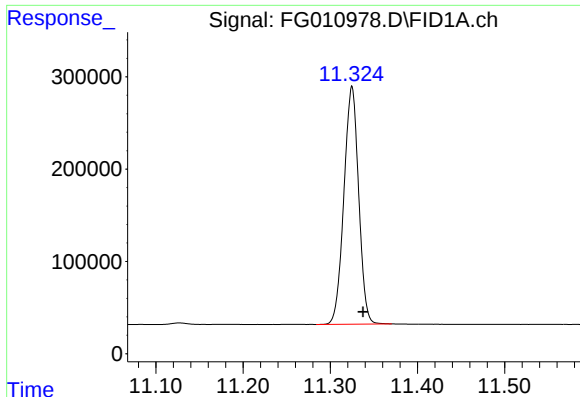

#6 N-OCTADECANE


R.T.: 11.325 min
Delta R.T.: -0.013 min
Response: 3028974
Conc: 21.49 ug/ml

Instrument :
FID_G
ClientSampleId :
PB148516BS

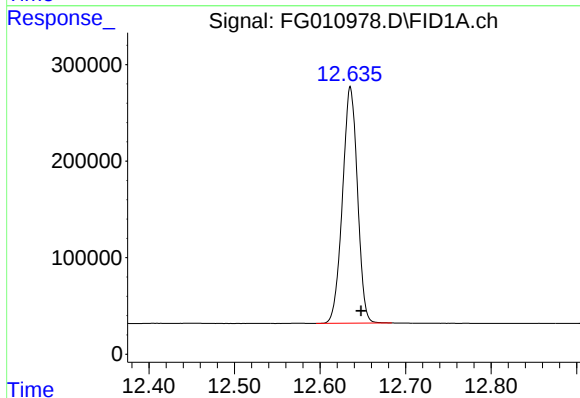


#7 N-EICOSANE

R.T.: 12.636 min
Delta R.T.: -0.012 min
Response: 2981957
Conc: 21.09 ug/ml

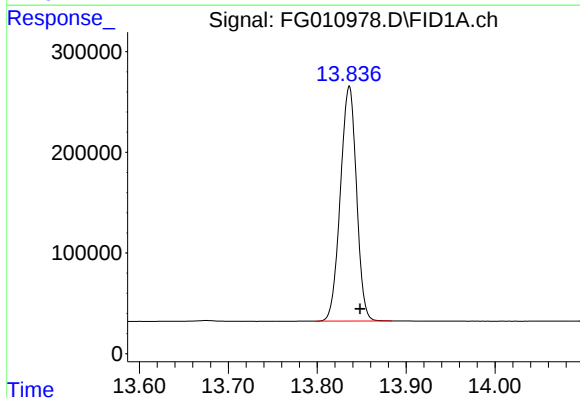


#8 N-DOCOSANE

R.T.: 13.836 min
Delta R.T.: -0.012 min
Response: 2941200
Conc: 21.25 ug/ml

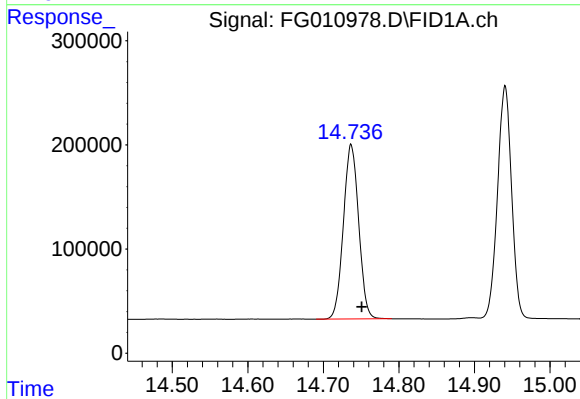

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.737 min
Delta R.T.: -0.014 min
Response: 2356088
Conc: 19.42 ug/ml

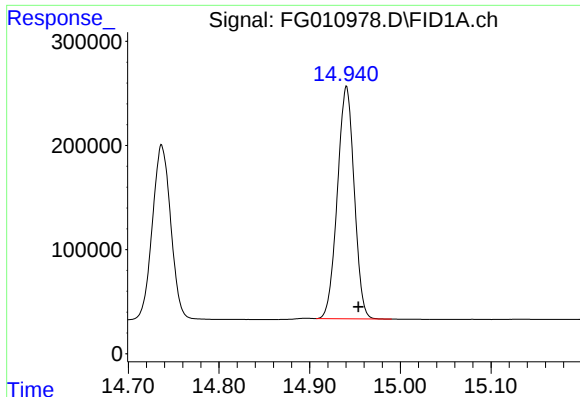

#10 N-TETRACOSANE


R.T.: 14.941 min
Delta R.T.: -0.013 min
Response: 2879341
Conc: 20.90 ug/ml

Instrument :
FID_G
ClientSampleId :
PB148516BS

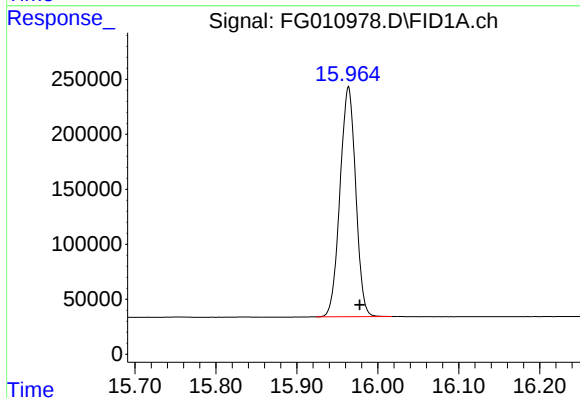

#11 N-HEXACOSANE

R.T.: 15.964 min
Delta R.T.: -0.014 min
Response: 2818352
Conc: 20.89 ug/ml

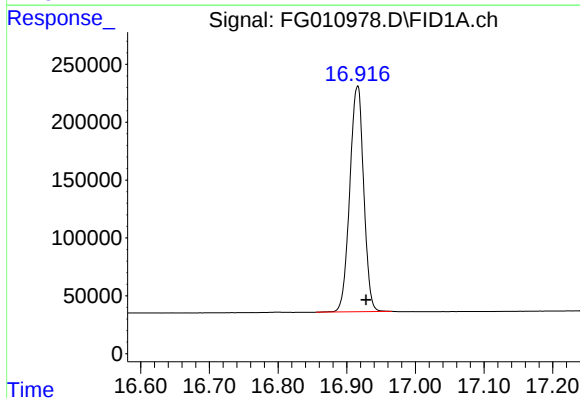

#12 N-OCTACOSANE

R.T.: 16.916 min
Delta R.T.: -0.013 min
Response: 2743524
Conc: 20.92 ug/ml