

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010981.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 15:47
Operator : YP\AJ
Sample : N5234-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LSP-SS-03-01-03-D

Integration File: autoint1.e
Quant Time: Oct 25 06:06:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.724	1688228	13.916 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010981.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 15:47
Operator : YP\AJ
Sample : N5234-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LSP-SS-03-01-03-D

Integration File: autoint1.e
Quant Time: Oct 25 06:06:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

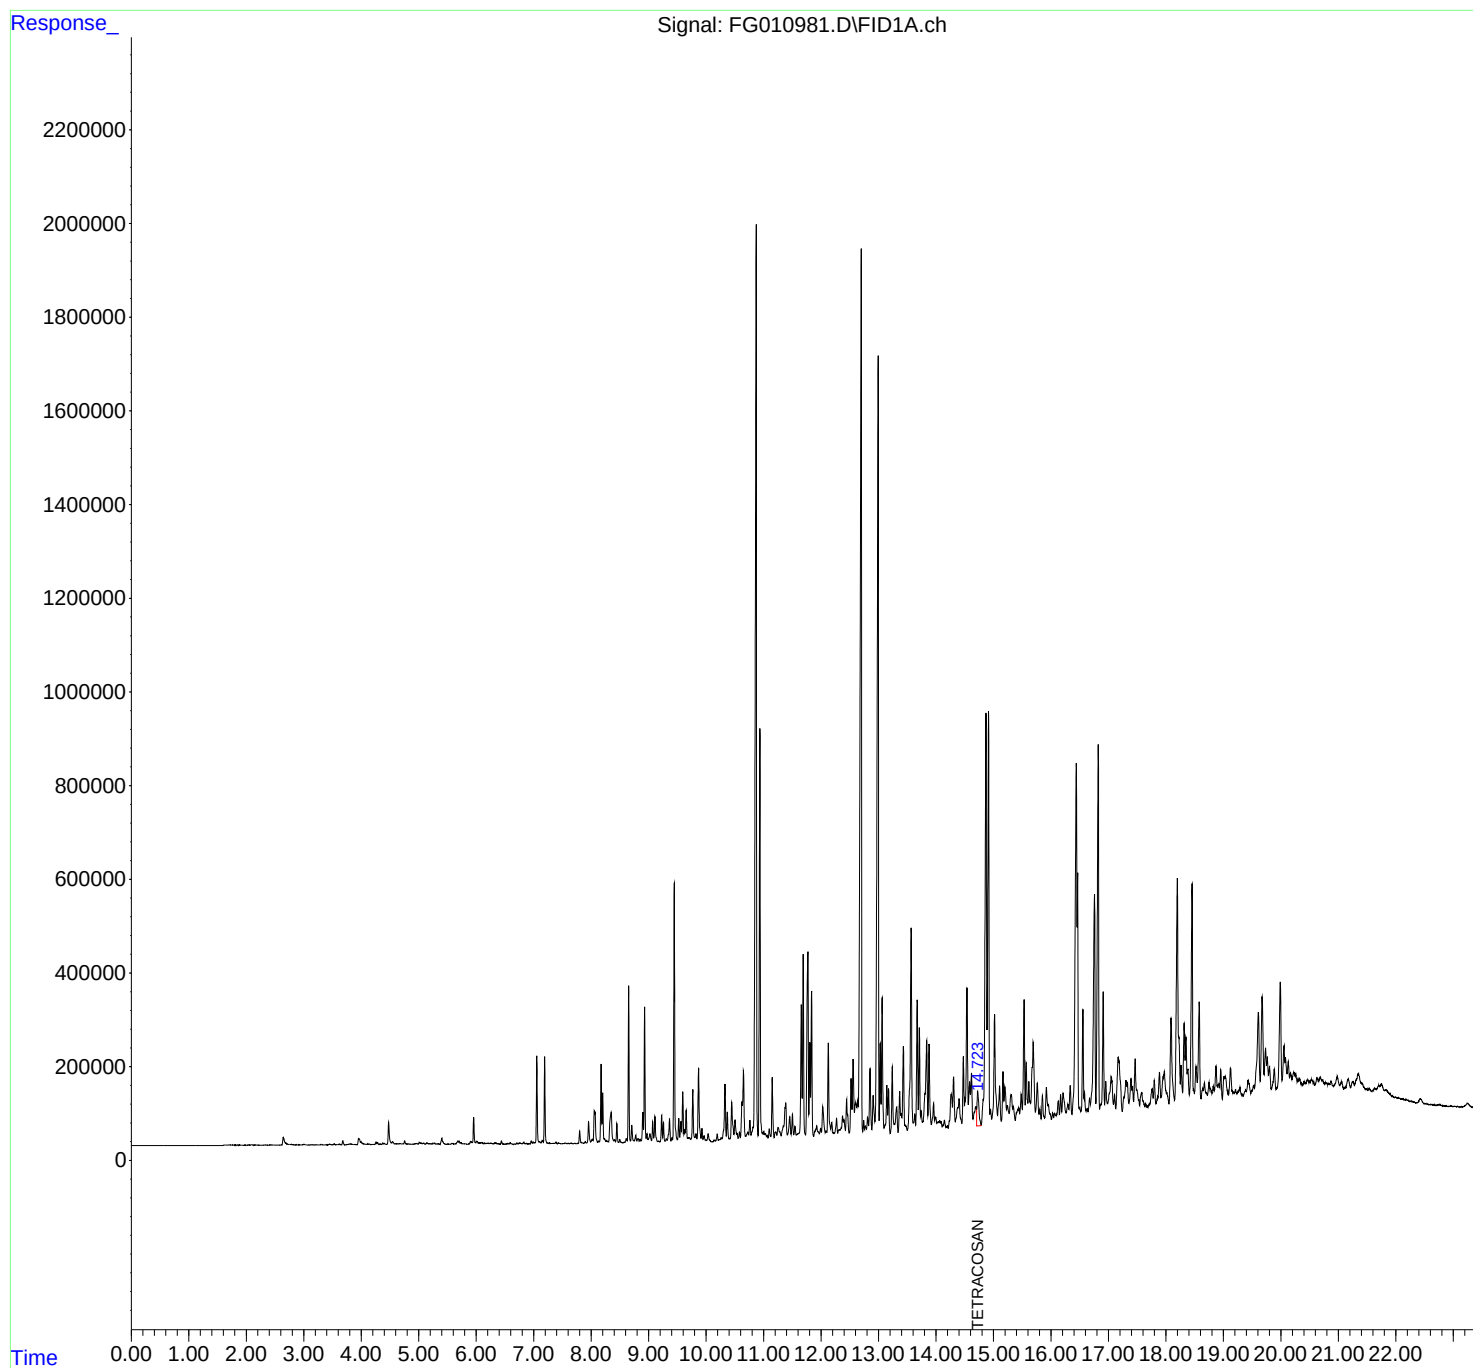

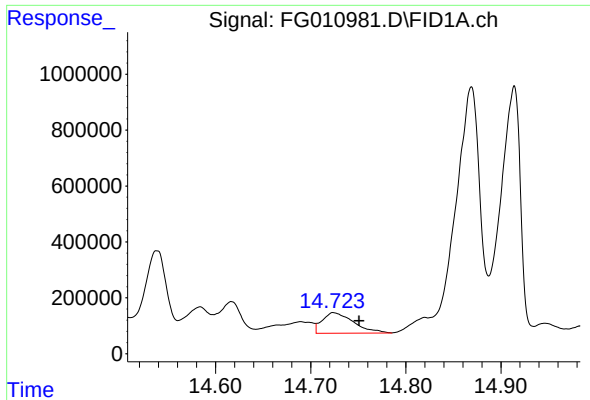

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.724 min
Delta R.T.: -0.027 min
Response: 1688228
Conc: 13.92 ug/ml

Instrument :
FID_G
ClientSampleId :
LSP-SS-03-01-03-D