

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
 Data File : FG010986.D
 Signal(s) : FID1A.ch
 Acq On : 24 Oct 2022 19:14
 Operator : YP\AJ
 Sample : N5234-06 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 LSP-SS-06-00-20

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/25/2022
 Supervised By :Ankita Jodhani 10/25/2022

Integration File: autoint1.e
 Quant Time: Oct 25 06:06:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
 Quant Title :
 QLast Update : Thu Sep 29 02:21:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.734	174717	1.440 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010986.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 19:14
Operator : YP\AJ
Sample : N5234-06 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
LSP-SS-06-00-20


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022

Integration File: autoint1.e
Quant Time: Oct 25 06:06:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

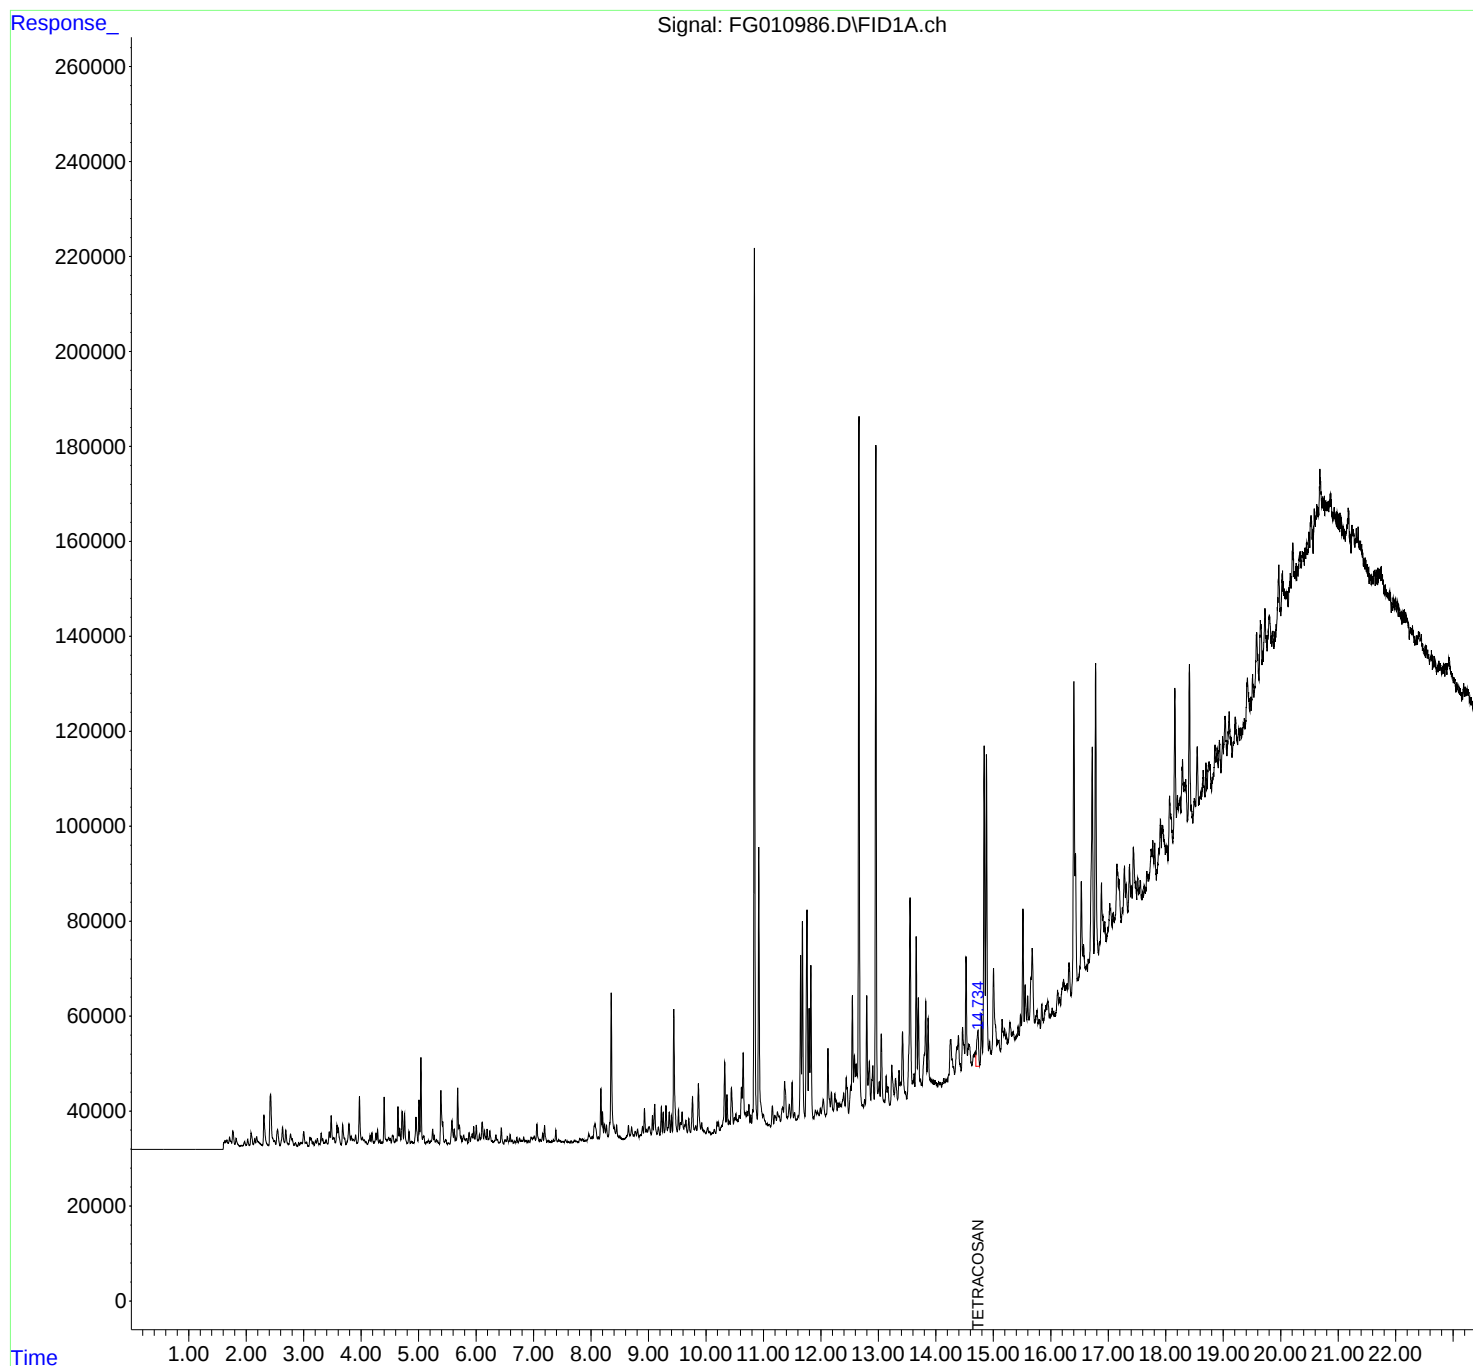

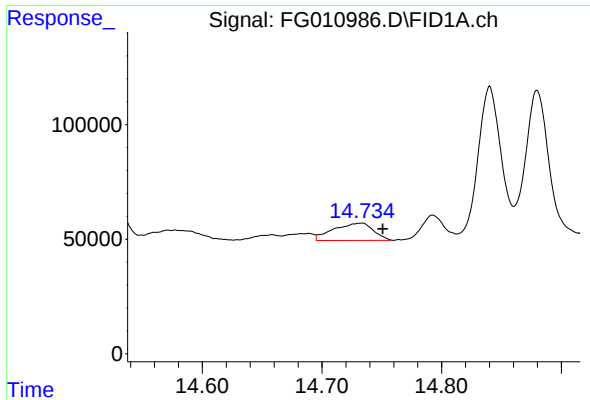

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.734 min
Delta R.T.: -0.017 min
Response: 174717
Conc: 1.44 ug/ml

Instrument :
FID_G
ClientSampleId :
LSP-SS-06-00-20

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022