

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010987.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 19:44
Operator : YP\AJ
Sample : N5234-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LSP-SS-06-20-40

Integration File: autoint1.e
Quant Time: Oct 25 06:07:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	1767496	14.569 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102422\
Data File : FG010987.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 19:44
Operator : YP\AJ
Sample : N5234-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LSP-SS-06-20-40

Integration File: autoint1.e
Quant Time: Oct 25 06:07:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

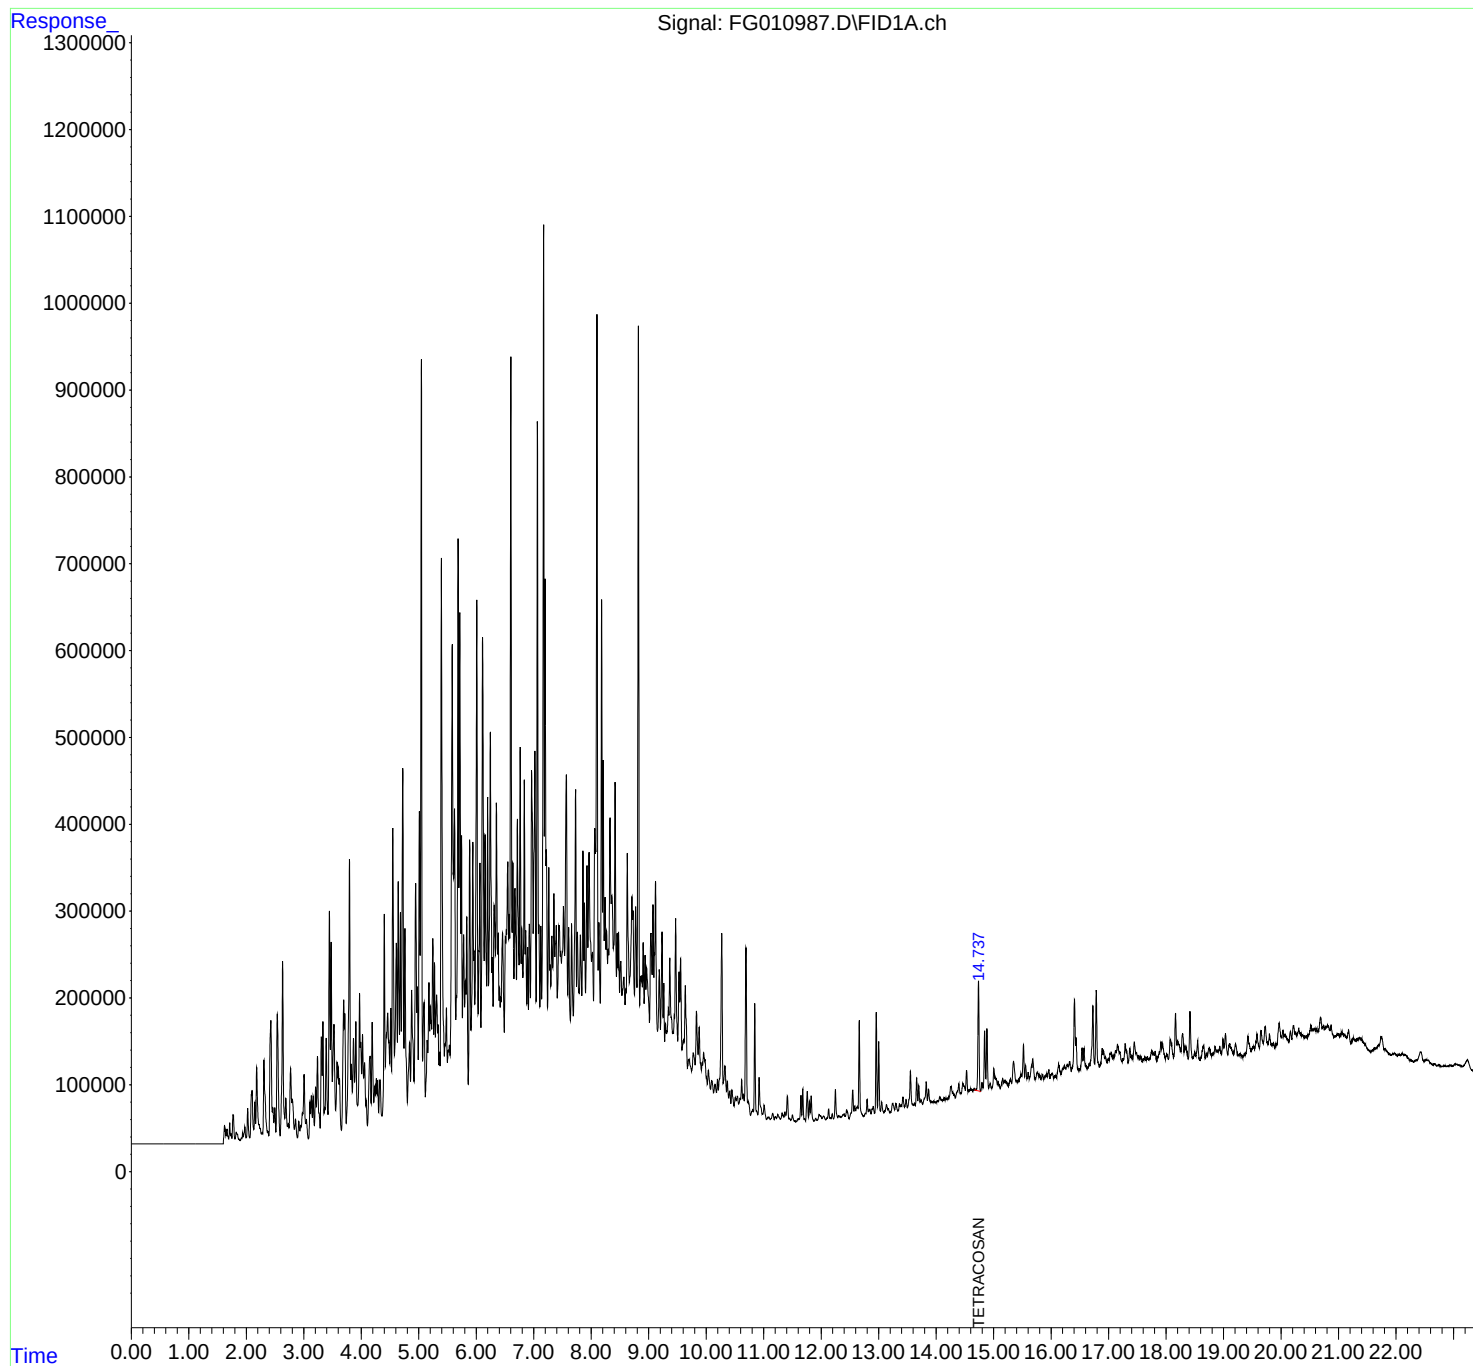

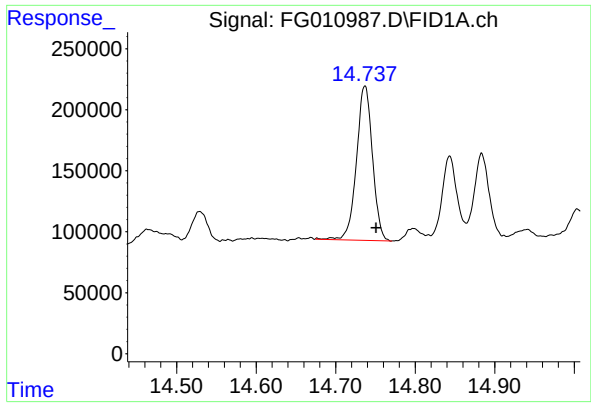

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: -0.014 min
Response: 1767496
Conc: 14.57 ug/ml

Instrument :
FID_G
ClientSampleId :
LSP-SS-06-20-40