

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102522\
Data File : FG010999.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2022 08:43
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2022
Supervised By :Ankita Jodhani 10/27/2022

Integration File: autoint1.e
Quant Time: Oct 26 04:57:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	2160798	17.811 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102522\
Data File : FG010999.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2022 08:43
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2022
Supervised By :Ankita Jodhani 10/27/2022

Integration File: autoint1.e
Quant Time: Oct 26 04:57:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

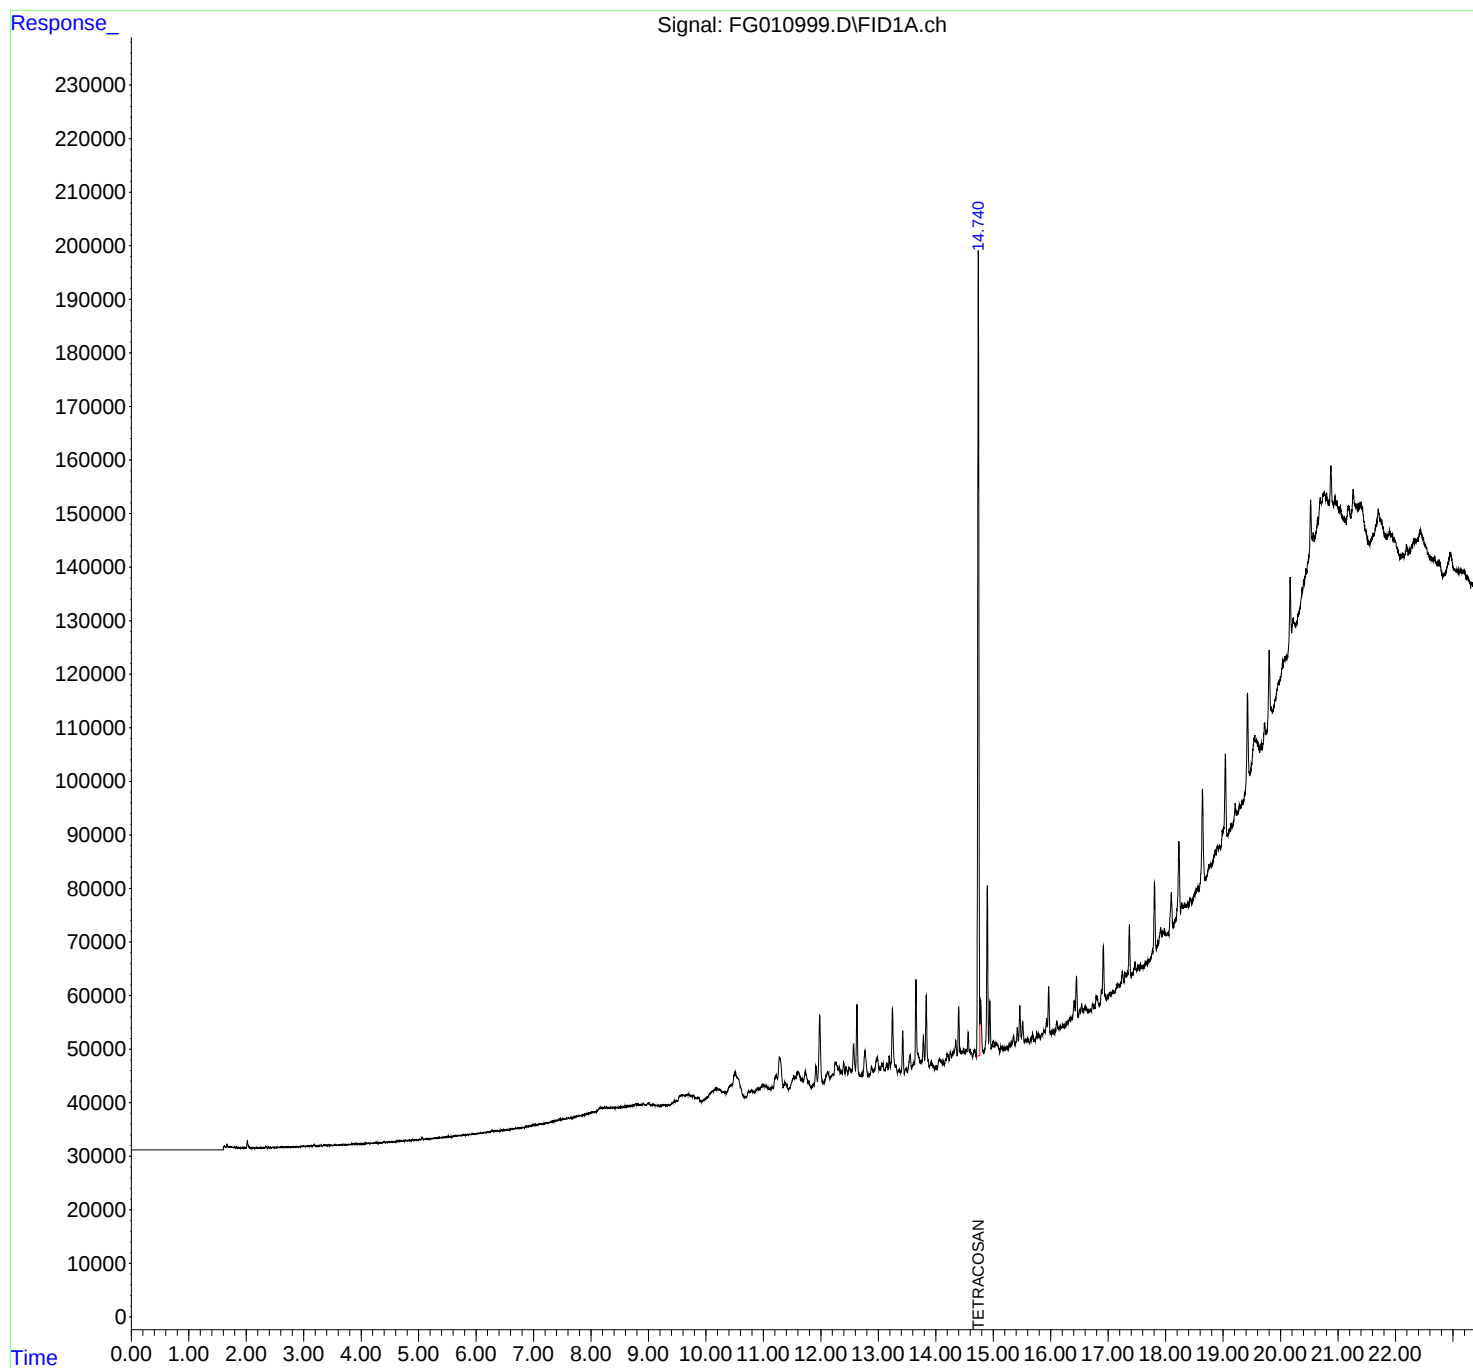

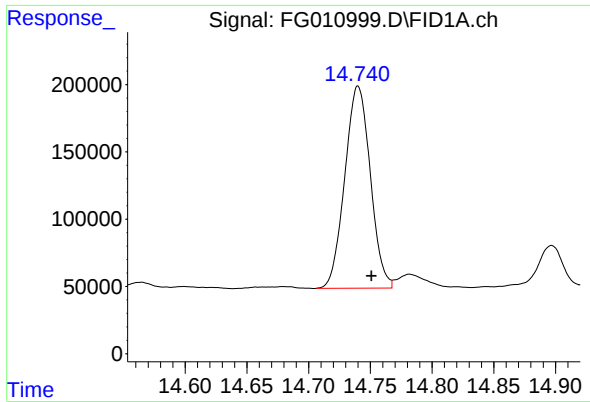

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: -0.011 min
Response: 2160798
Conc: 17.81 ug/ml

Instrument :

FID_G

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 10/27/2022
Supervised By :Ankita Jodhani 10/27/2022