

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102522\
 Data File : FG011000.D
 Signal(s) : FID1A.ch
 Acq On : 25 Oct 2022 09:12
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Oct 26 04:57:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
 Quant Title :
 QLast Update : Thu Sep 29 02:21:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.742	5822588	47.994 ug/ml
Target Compounds			
2) N-DECANE	4.260	7242442	55.652 ug/ml
3) N-DODECANE	6.443	7352774	55.442 ug/ml
4) N-TETRADECANE	8.275	7308772	54.506 ug/ml
5) N-HEXADECANE	9.884	7397954	53.354 ug/ml
6) N-OCTADECANE	11.329	7388502	52.424 ug/ml
7) N-EICOSANE	12.641	7241665	51.210 ug/ml
8) N-DOCOSANE	13.841	6924378	50.020 ug/ml
10) N-TETRACOSANE	14.945	6831094	49.582 ug/ml
11) N-HEXACOSANE	15.969	6632687	49.163 ug/ml
12) N-OCTACOSANE	16.922	6573793	50.130 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102522\
Data File : FG011000.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2022 09:12
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Oct 26 04:57:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

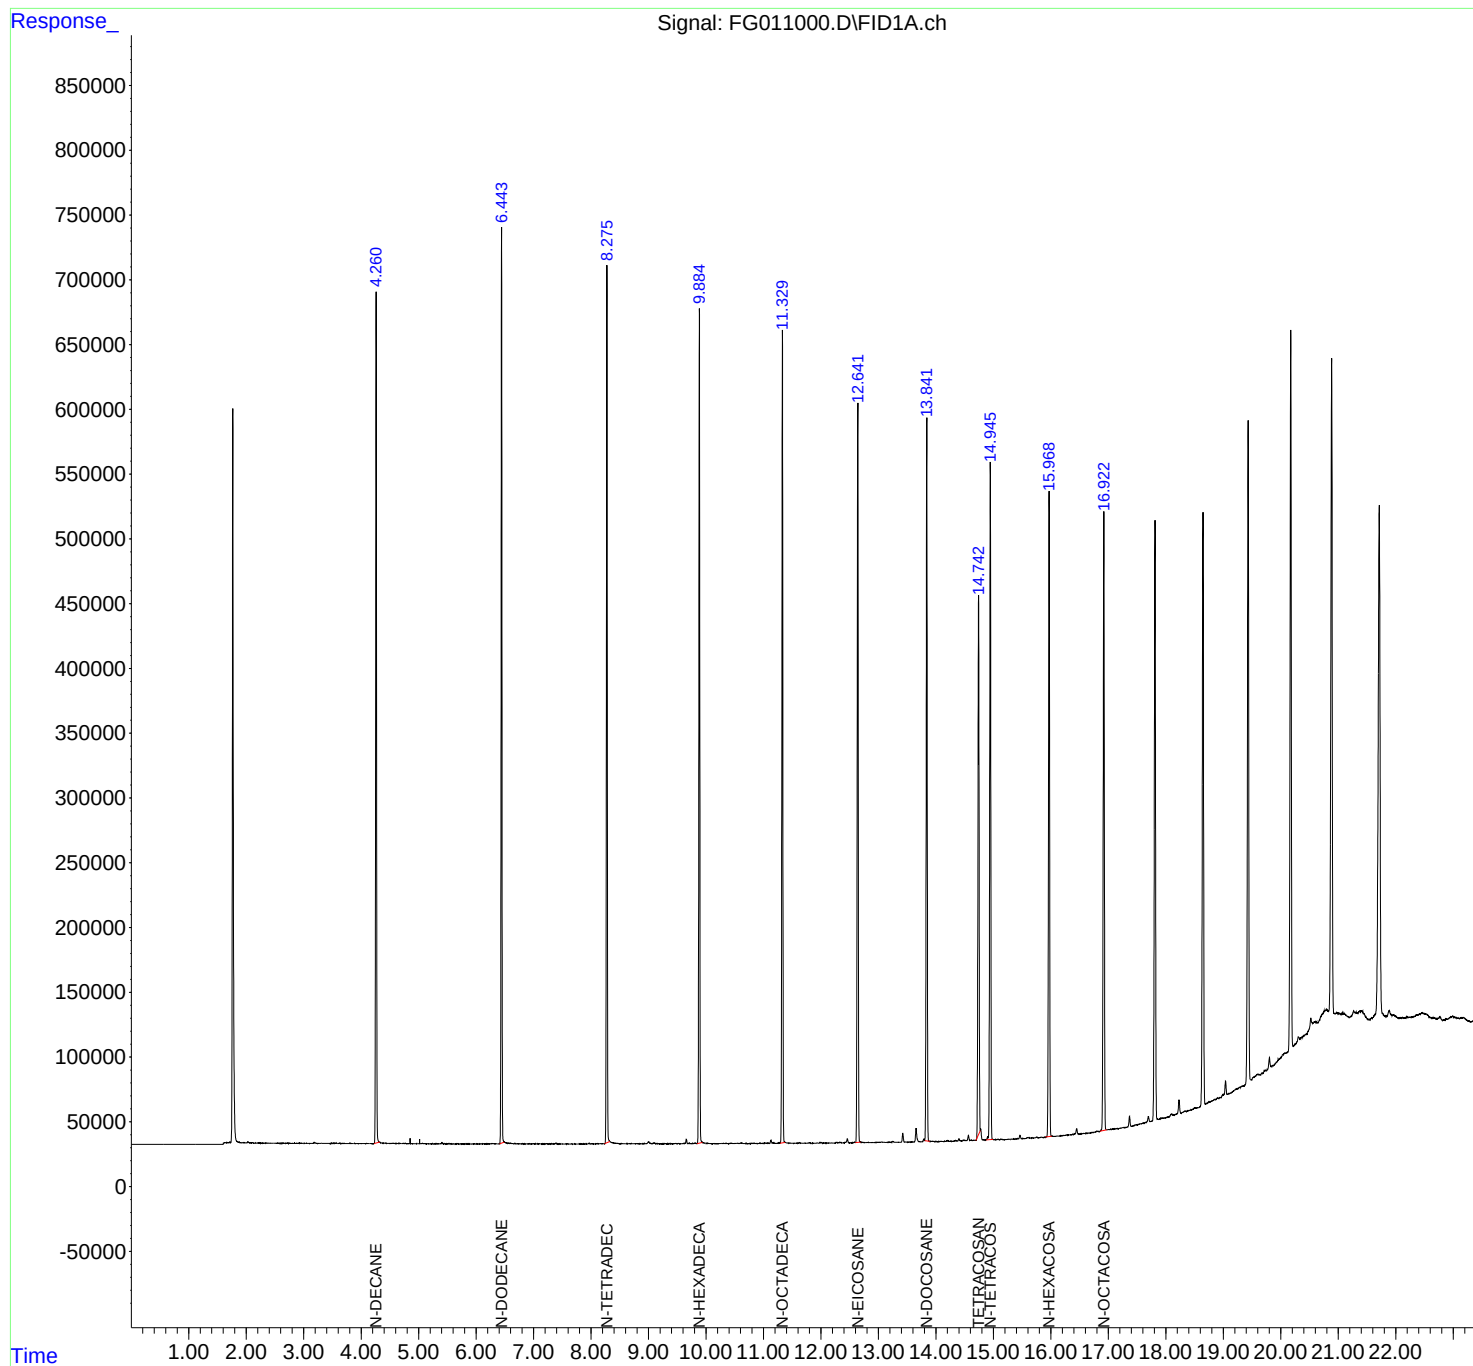


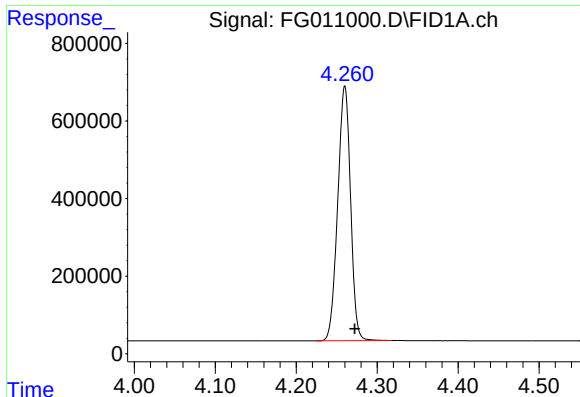

#2 N-DECANE


R.T.: 4.260 min
Delta R.T.: -0.012 min
Response: 7242442
Conc: 55.65 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

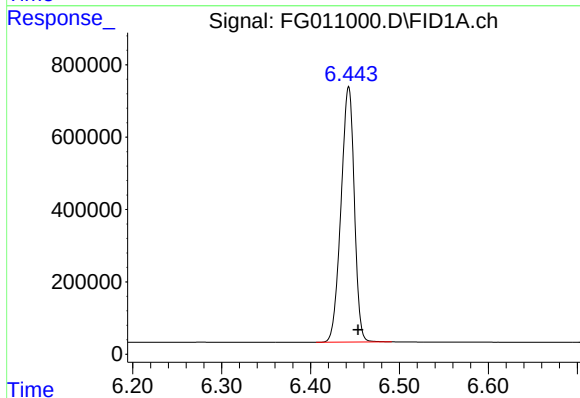


#3 N-DODECANE

R.T.: 6.443 min
Delta R.T.: -0.011 min
Response: 7352774
Conc: 55.44 ug/ml

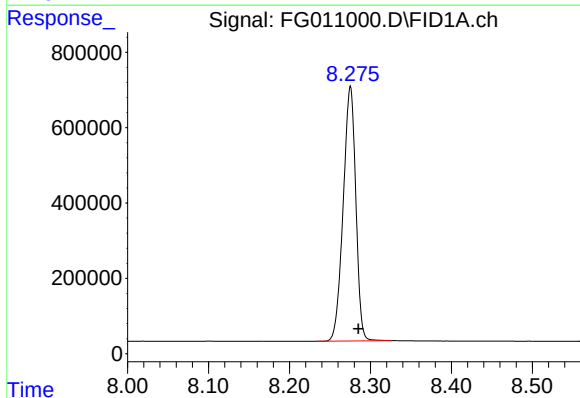


#4 N-TETRADECANE

R.T.: 8.275 min
Delta R.T.: -0.010 min
Response: 7308772
Conc: 54.51 ug/ml

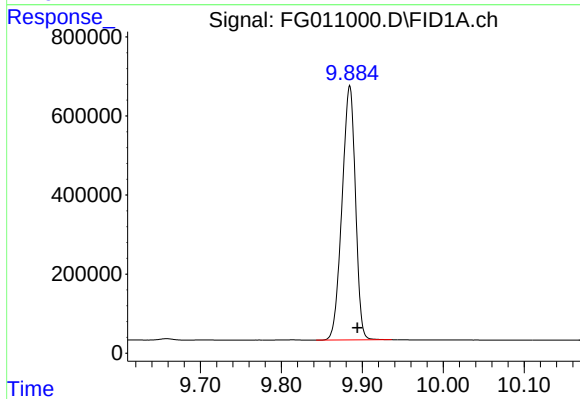

#5 N-HEXADECANE


R.T.: 9.884 min
Delta R.T.: -0.009 min
Response: 7397954
Conc: 53.35 ug/ml

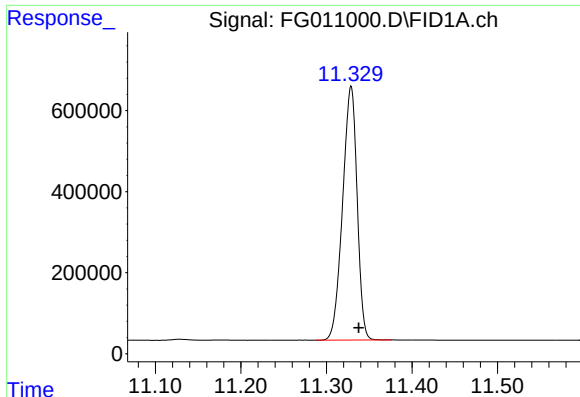

#6 N-OCTADECANE


R.T.: 11.329 min
Delta R.T.: -0.009 min
Response: 7388502
Conc: 52.42 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

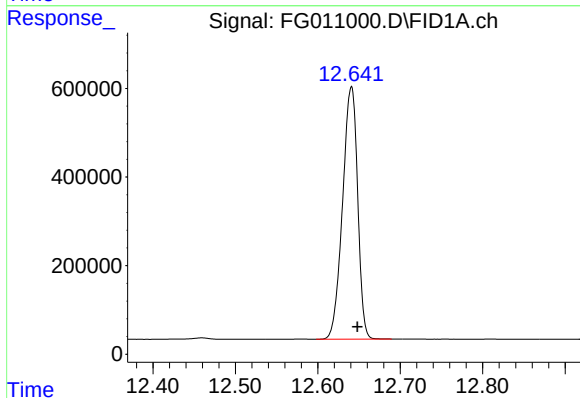


#7 N-EICOSANE

R.T.: 12.641 min
Delta R.T.: -0.007 min
Response: 7241665
Conc: 51.21 ug/ml

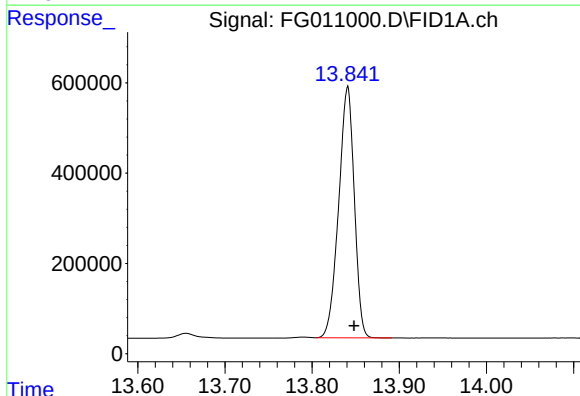


#8 N-DOCOSANE

R.T.: 13.841 min
Delta R.T.: -0.008 min
Response: 6924378
Conc: 50.02 ug/ml

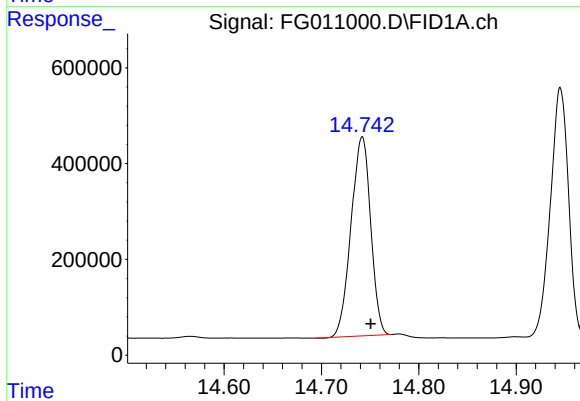

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.742 min
Delta R.T.: -0.009 min
Response: 5822588
Conc: 47.99 ug/ml

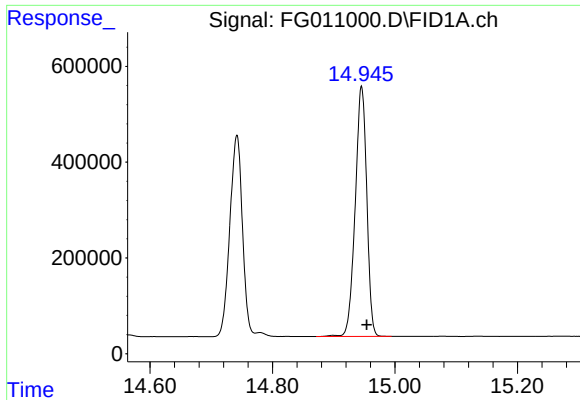

#10 N-TETRACOSANE


R.T.: 14.945 min
Delta R.T.: -0.008 min
Response: 6831094
Conc: 49.58 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

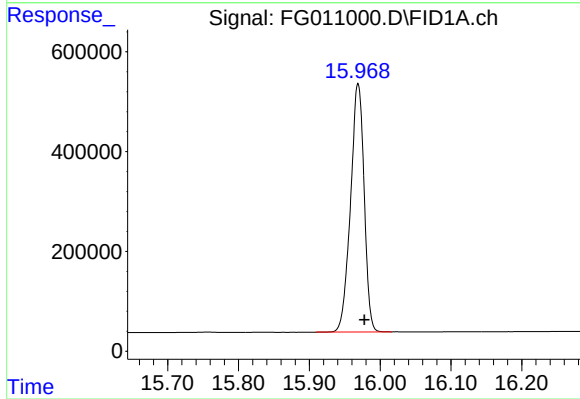

#11 N-HEXACOSANE

R.T.: 15.969 min
Delta R.T.: -0.009 min
Response: 6632687
Conc: 49.16 ug/ml

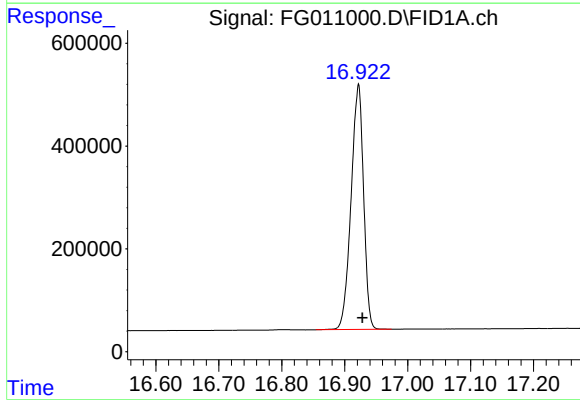

#12 N-OCTACOSANE

R.T.: 16.922 min
Delta R.T.: -0.006 min
Response: 6573793
Conc: 50.13 ug/ml