

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102522\
Data File : FG011006.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2022 12:10
Operator : YP\AJ
Sample : N5235-01 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LSP-SS-01-00-20

Integration File: autoint1.e
Quant Time: Oct 26 04:58:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	322457	2.658 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102522\
Data File : FG011006.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2022 12:10
Operator : YP\AJ
Sample : N5235-01 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LSP-SS-01-00-20

Integration File: autoint1.e
Quant Time: Oct 26 04:58:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

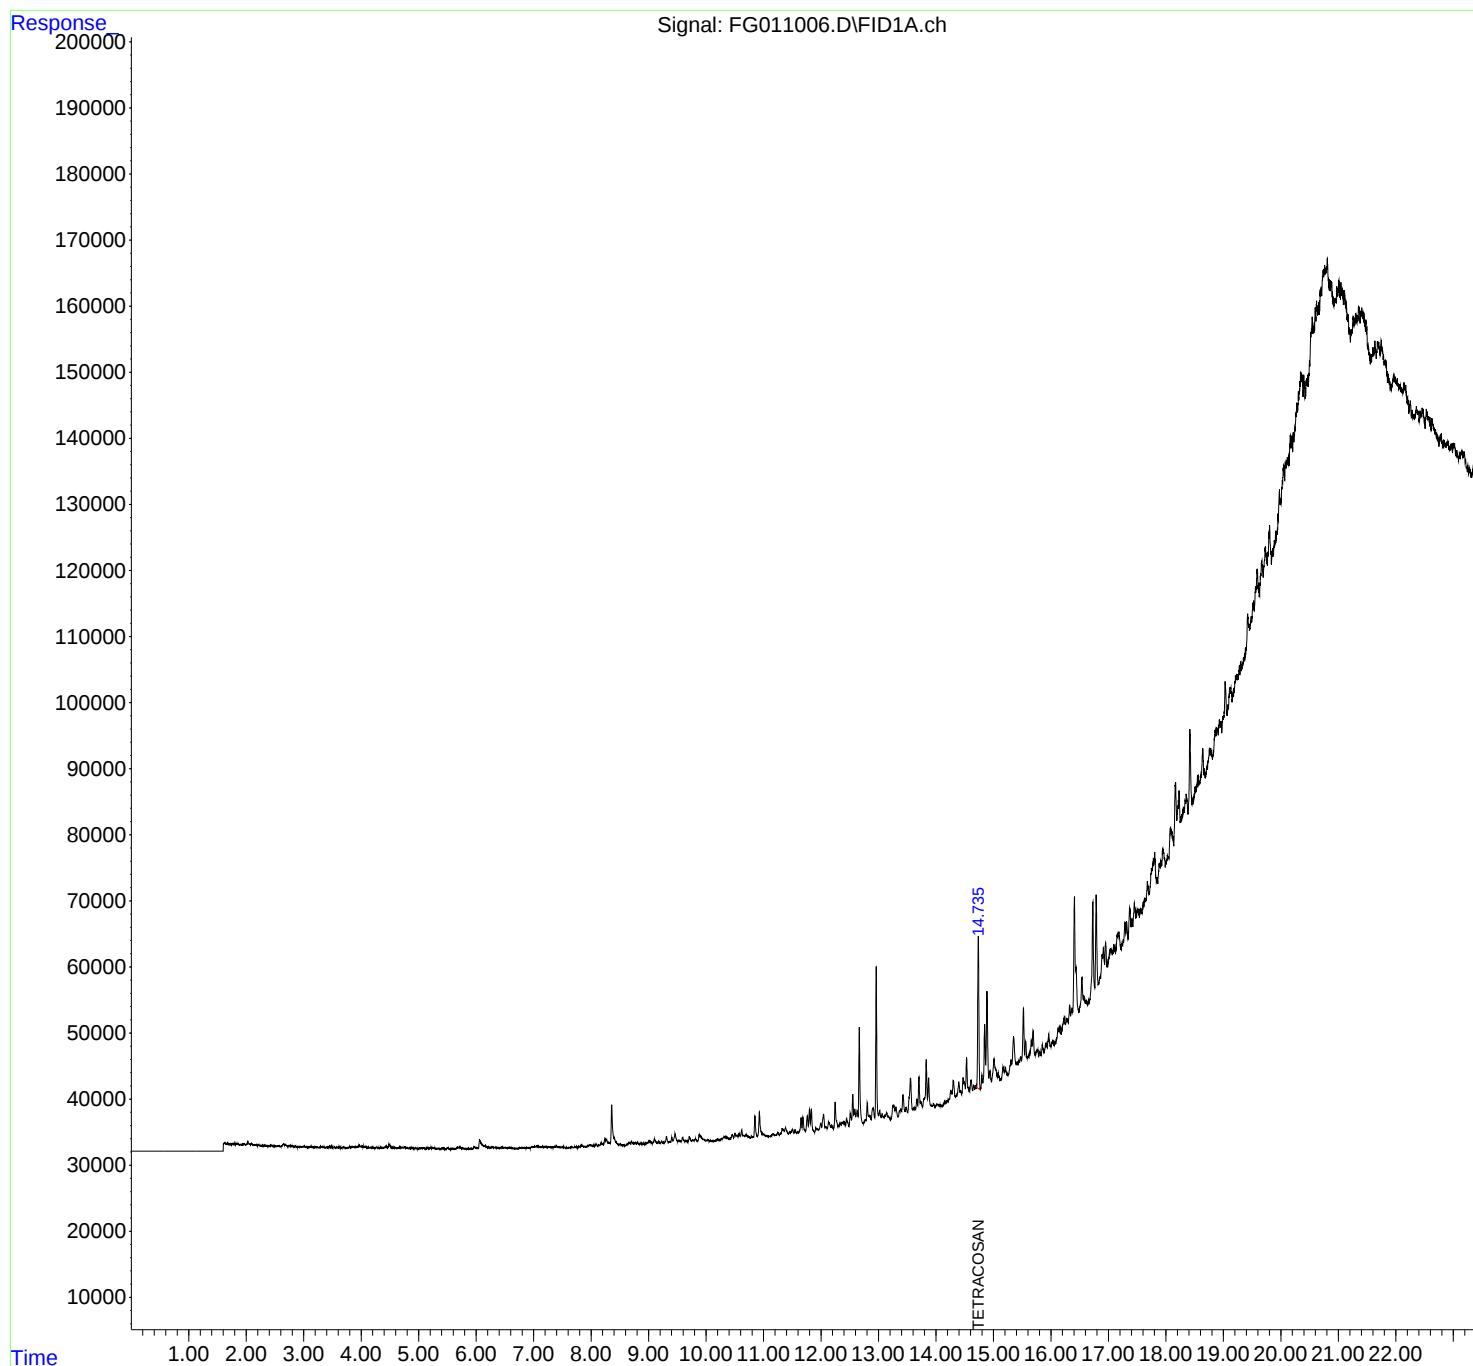

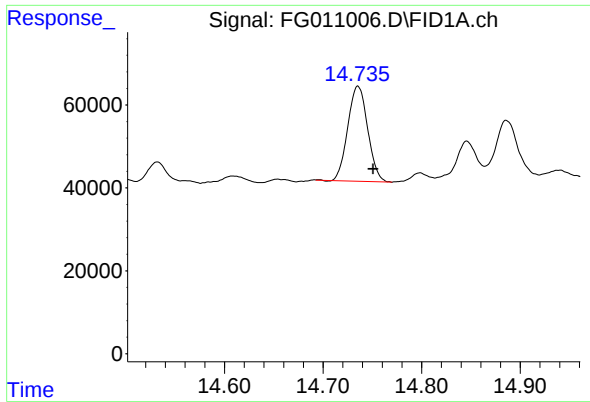

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.735 min
Delta R.T.: -0.015 min
Response: 322457
Conc: 2.66 ug/ml

Instrument :
FID_G
ClientSampleId :
LSP-SS-01-00-20