

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102622\
Data File : FG011016.D
Signal(s) : FID1A.ch
Acq On : 26 Oct 2022 08:20
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 26 11:40:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.436	1390693	10.486 ug/ml
12) N-OCTACOSANE	16.908	1481815	11.300 ug/ml
13) N-TRIACONTANE	17.797	327996	2.548 ug/ml
14) N-DOTRIACONTANE	18.632	433824	3.414 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102622\
Data File : FG011016.D
Signal(s) : FID1A.ch
Acq On : 26 Oct 2022 08:20
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 26 11:40:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

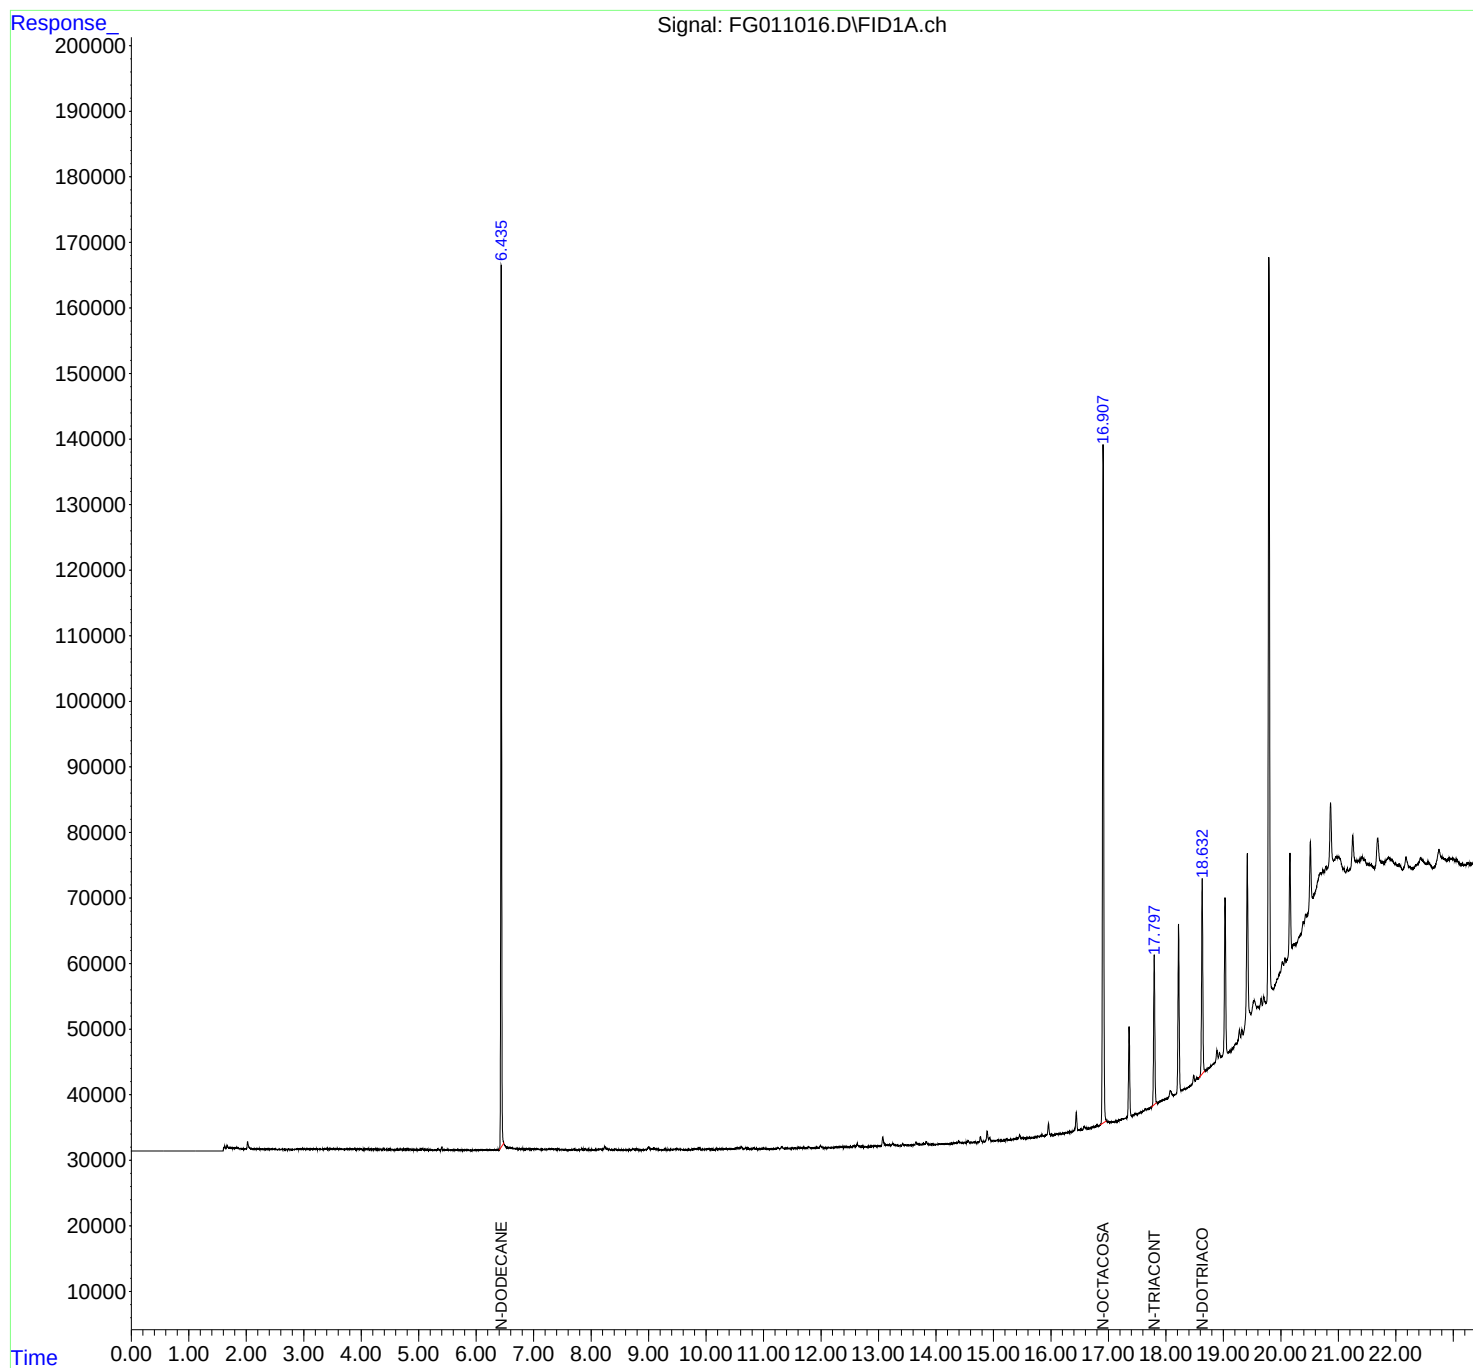


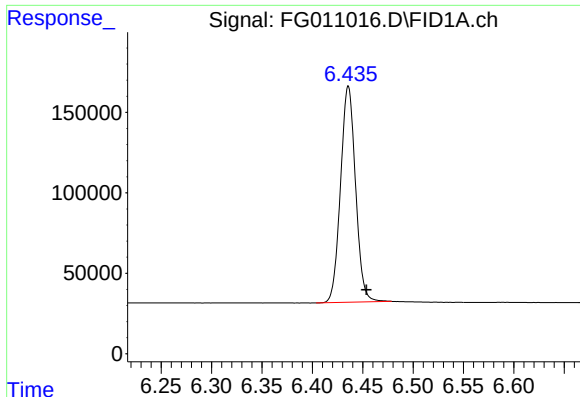

#3 N-DODECANE


R.T.: 6.436 min
Delta R.T.: -0.018 min
Response: 1390693
Conc: 10.49 ug/ml

Instrument :
FID_G
ClientSampleId :

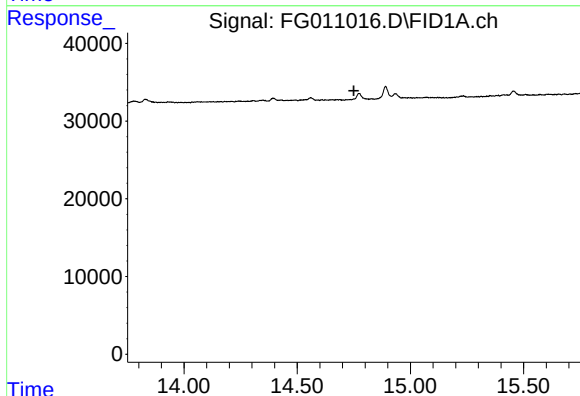


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.751 min
Response: 0
Conc: N.D.

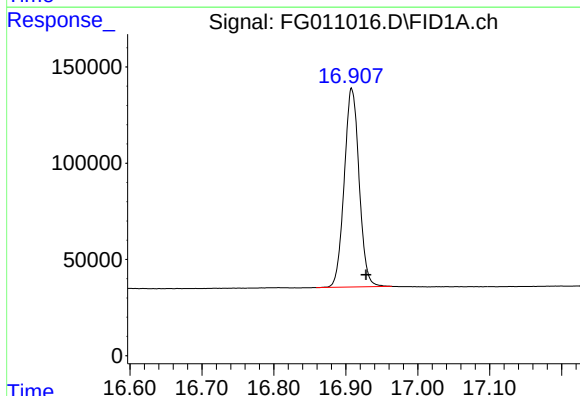


#12 N-OCTACOSANE

R.T.: 16.908 min
Delta R.T.: -0.020 min
Response: 1481815
Conc: 11.30 ug/ml

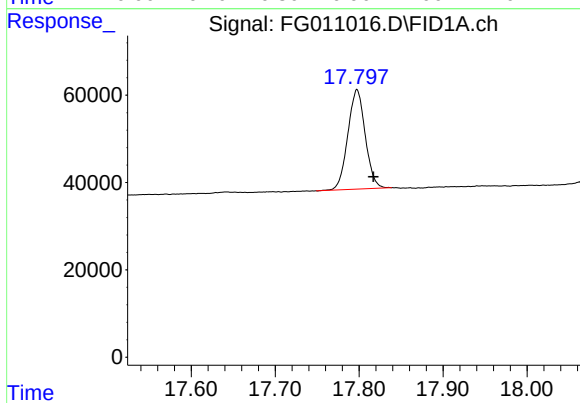

#13 N-TRIACONTANE

R.T.: 17.797 min
Delta R.T.: -0.020 min
Response: 327996
Conc: 2.55 ug/ml

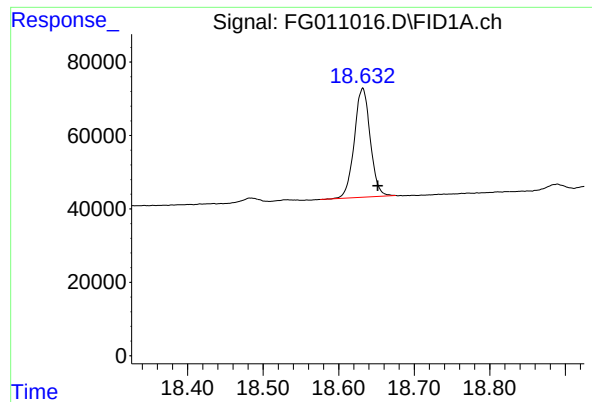

#14 N-DOTRIACONTANE

R.T.: 18.632 min
Delta R.T.: -0.020 min
Response: 433824
Conc: 3.41 ug/ml

Instrument :

FID_G

ClientSampleId :