

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102622\
Data File : FG011027.D
Signal(s) : FID1A.ch
Acq On : 26 Oct 2022 14:18
Operator : YP\AJ
Sample : PB148504BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB148504BL

Integration File: Sample.e
Quant Time: Oct 27 04:52:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.729	2587523	21.328 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102622\
Data File : FG011027.D
Signal(s) : FID1A.ch
Acq On : 26 Oct 2022 14:18
Operator : YP\AJ
Sample : PB148504BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB148504BL

Integration File: Sample.e
Quant Time: Oct 27 04:52:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

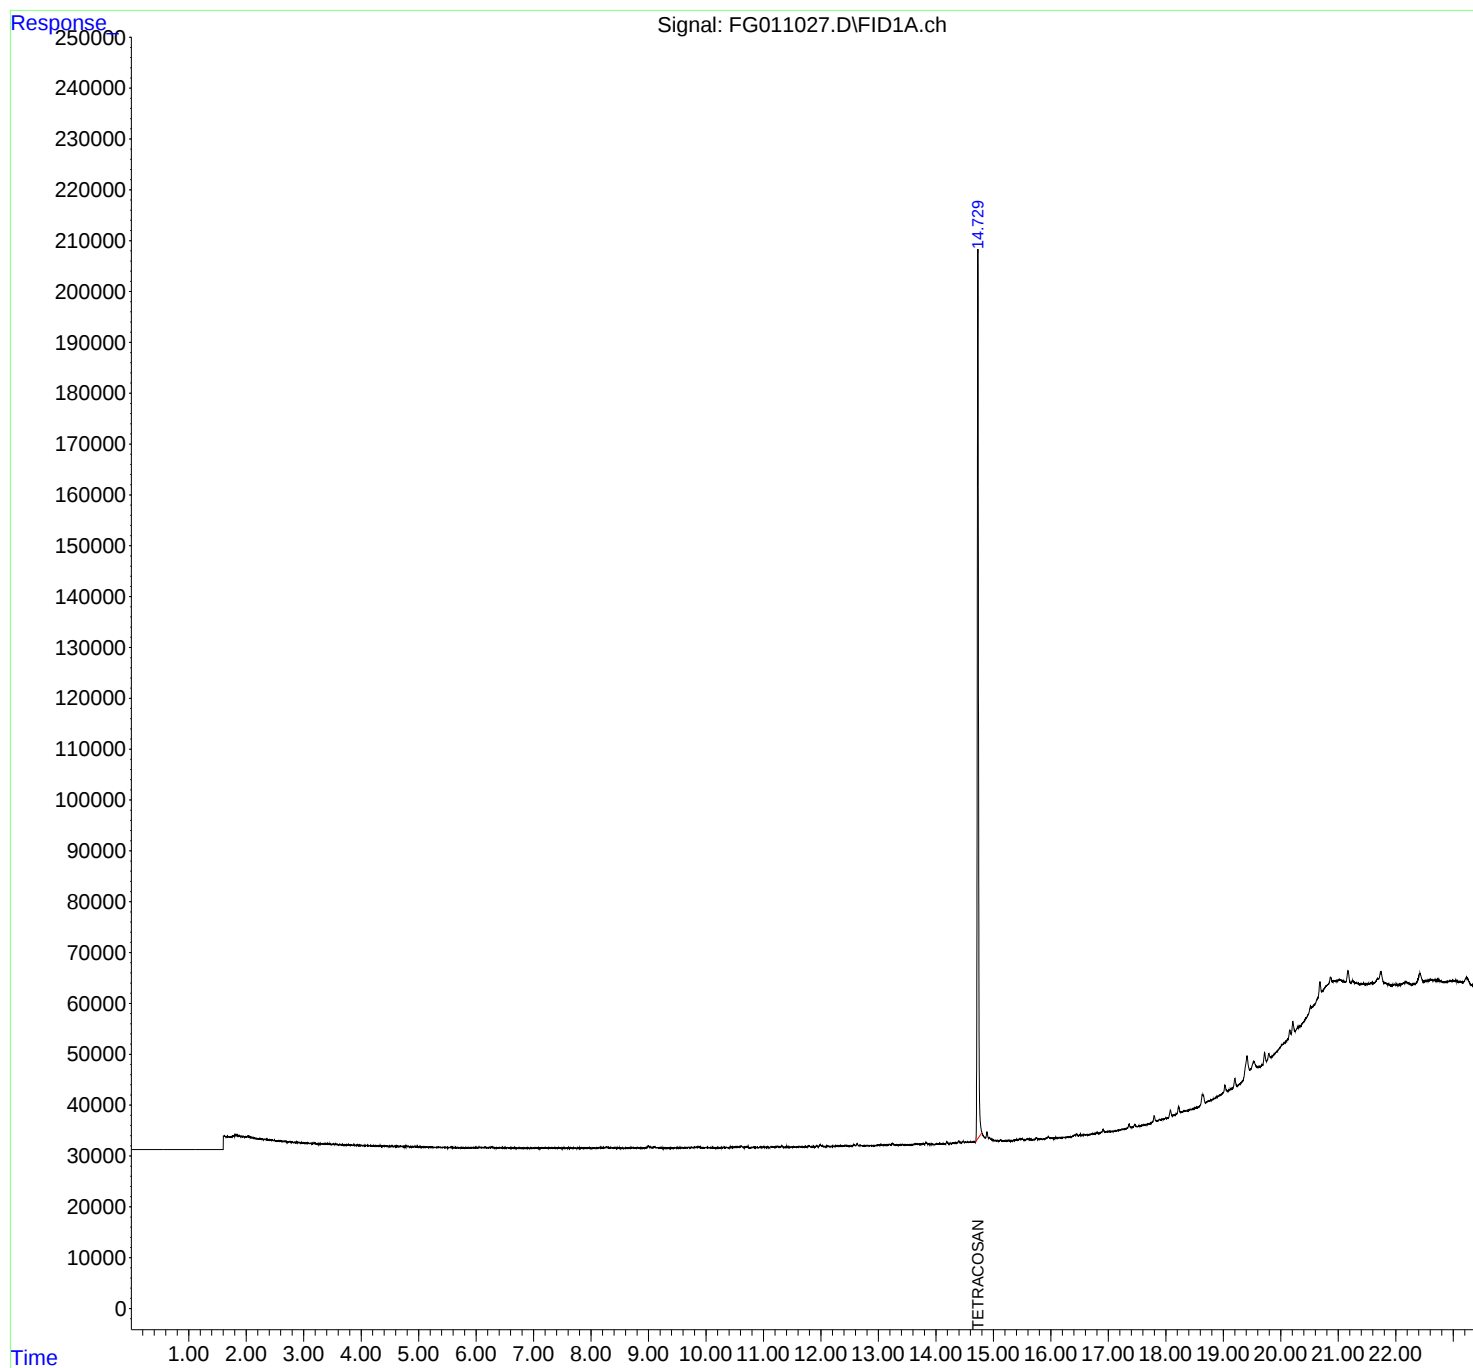

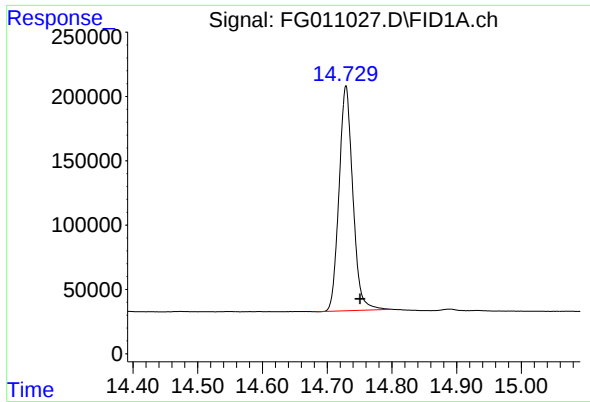

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.729 min
Delta R.T.: -0.022 min
Response: 2587523
Conc: 21.33 ug/ml

Instrument :
FID_G
ClientSampleId :
PB148504BL