

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102720\
 Data File : FF007764.D
 Signal(s) : FID2B.ch
 Acq On : 27 Oct 2020 12:08
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 28 00:57:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.466	5859622	40.552 ug/ml
12) N-OCTACOSANE	16.912	5278901	39.414 ug/ml
13) N-TRIACONTANE	17.799	460758	3.563 ug/ml
14) N-DOTRIACONTANE	18.633	550640	4.576 ug/ml
15) N-TETRATRIACONTANE	19.420	409467	3.897 ug/ml
16) N-HEXATRIACONTANE	20.163	241926	2.536 ug/ml
17) N-OCTATRIACONTANE	20.918	150050	1.816 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102720\
Data File : FF007764.D
Signal(s) : FID2B.ch
Acq On : 27 Oct 2020 12:08
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 28 00:57:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

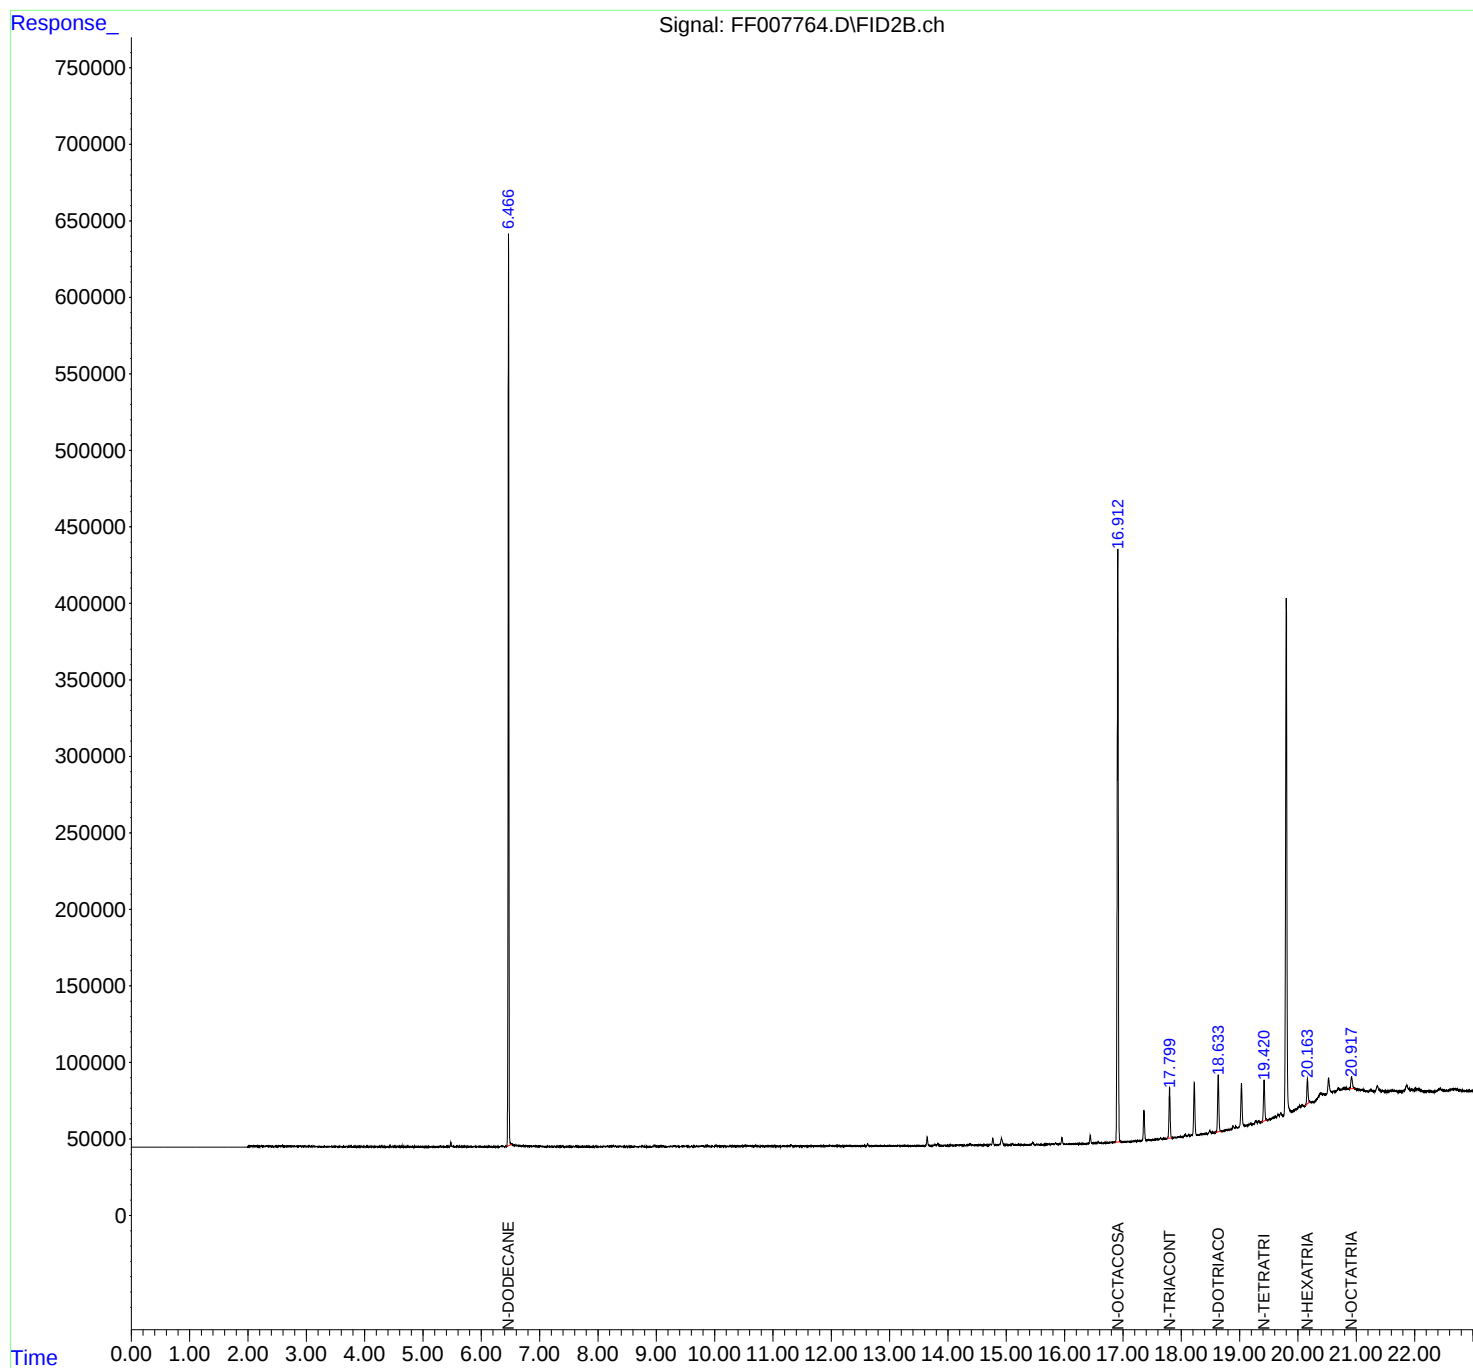


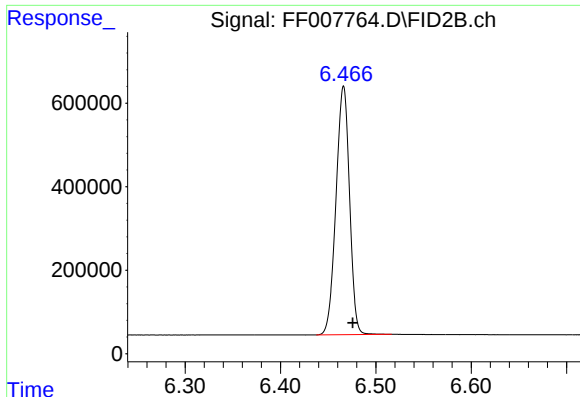

#3 N-DODECANE


R.T.: 6.466 min
Delta R.T.: -0.009 min
Response: 5859622
Conc: 40.55 ug/ml

Instrument :
FID_G
ClientSampleId :

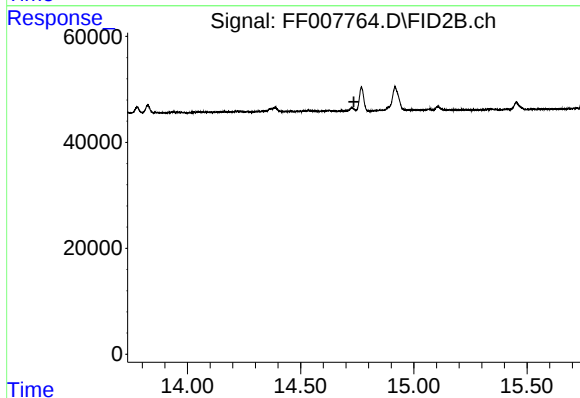


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.735 min
Response: 0
Conc: N.D.

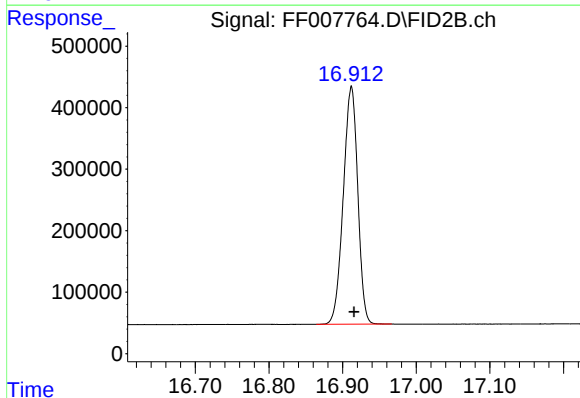


#12 N-OCTACOSANE

R.T.: 16.912 min
Delta R.T.: -0.004 min
Response: 5278901
Conc: 39.41 ug/ml

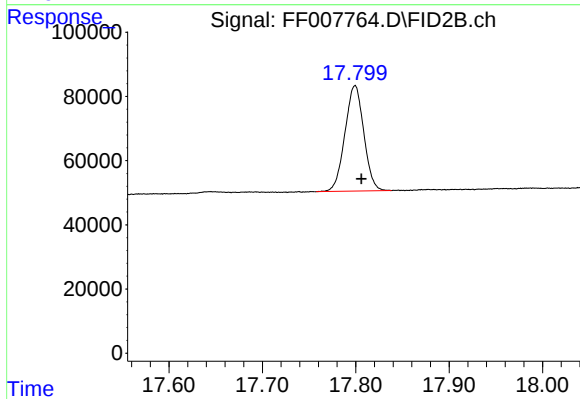

#13 N-TRIACONTANE


R.T.: 17.799 min
Delta R.T.: -0.007 min
Response: 460758
Conc: 3.56 ug/ml

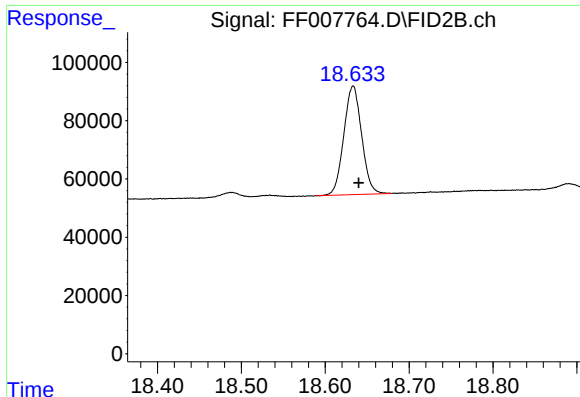

#14 N-DOTRIACONTANE


R.T.: 18.633 min
Delta R.T.: -0.006 min
Response: 550640
Conc: 4.58 ug/ml

Instrument :
FID_G
ClientSampleId :

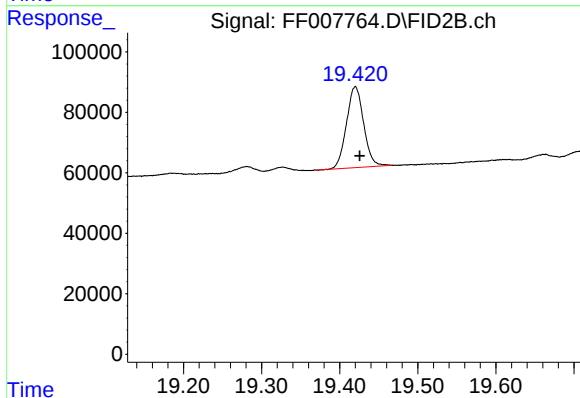


#15 N-TETRATRIACONTANE

R.T.: 19.420 min
Delta R.T.: -0.006 min
Response: 409467
Conc: 3.90 ug/ml

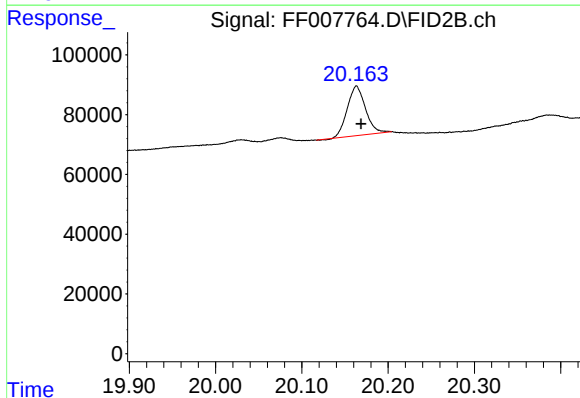

#16 N-HEXATRIACONTANE

R.T.: 20.163 min
Delta R.T.: -0.005 min
Response: 241926
Conc: 2.54 ug/ml

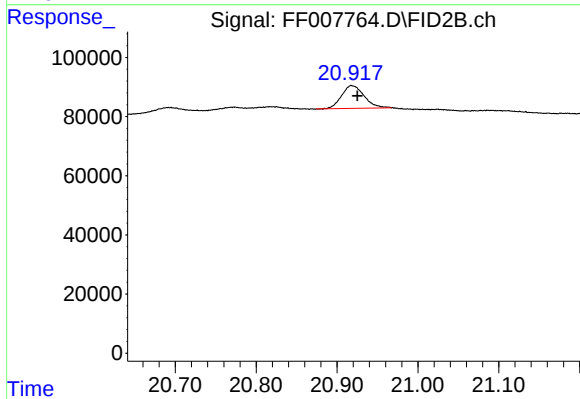

#17 N-OCTATRIACONTANE

R.T.: 20.918 min
Delta R.T.: -0.007 min
Response: 150050
Conc: 1.82 ug/ml