

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102720\
 Data File : FF007765.D
 Signal(s) : FID2B.ch
 Acq On : 27 Oct 2020 12:53
 Operator : DD\AJ
 Sample : L4513-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 28 00:57:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.728	1112929	8.843 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.226	267358	1.834 ug/ml
10)	N-TETRACOSANE	14.919	145925	1.012 ug/ml
14)	N-DOTRIACONTANE	18.633	89217	0.741 ug/ml
15)	N-TETRATRIACONTANE	19.490f	76444	0.728 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102720\
Data File : FF007765.D
Signal(s) : FID2B.ch
Acq On : 27 Oct 2020 12:53
Operator : DD\AJ
Sample : L4513-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 28 00:57:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

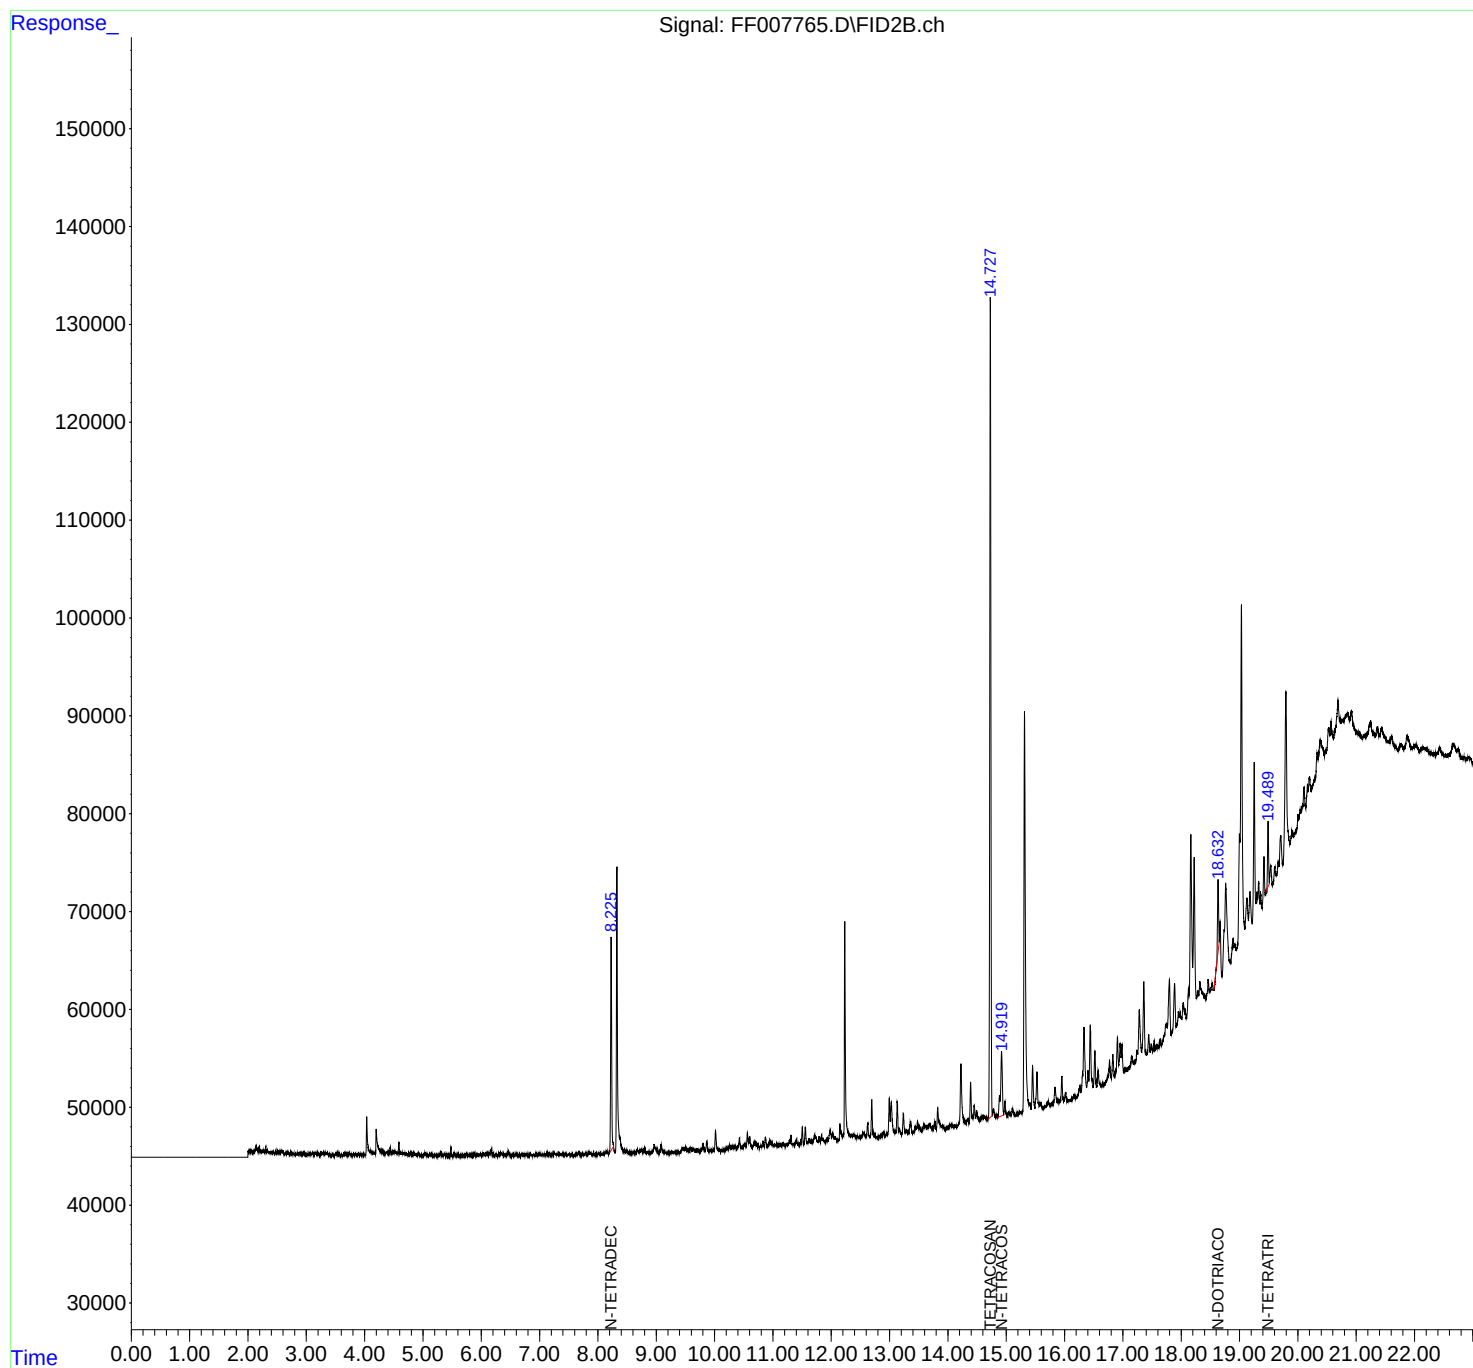


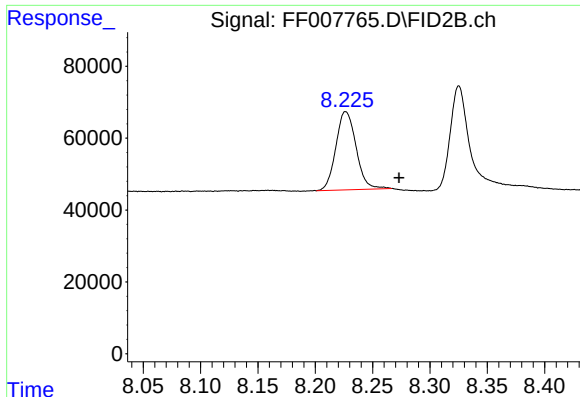

#4 N-TETRADECANE


R.T.: 8.226 min
Delta R.T.: -0.047 min
Response: 267358
Conc: 1.83 ug/ml

Instrument :
FID_G
ClientSampleId :

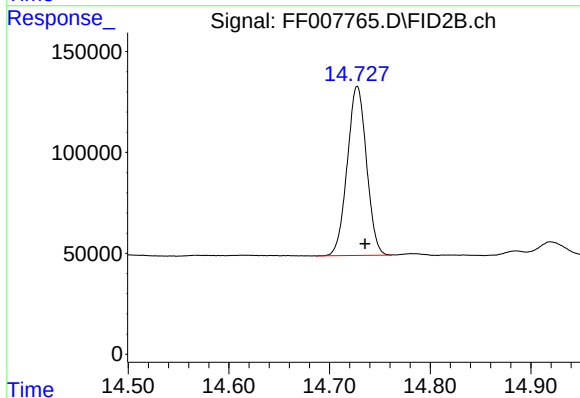


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.728 min
Delta R.T.: -0.008 min
Response: 1112929
Conc: 8.84 ug/ml

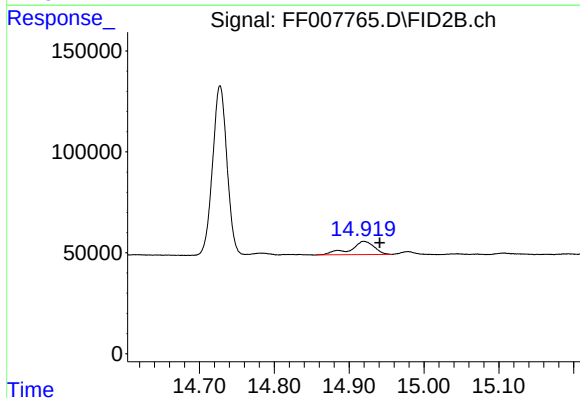


#10 N-TETRACOSANE

R.T.: 14.919 min
Delta R.T.: -0.021 min
Response: 145925
Conc: 1.01 ug/ml

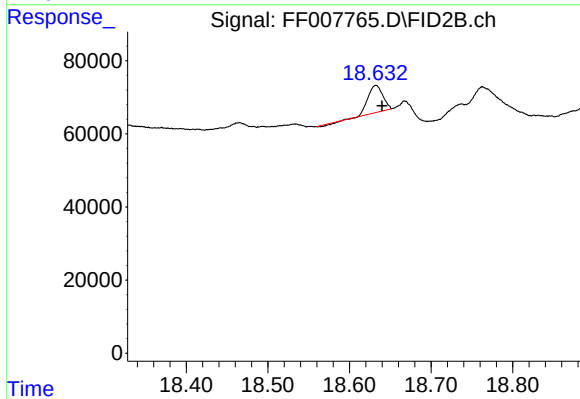

#14 N-DOTRIACONTANE

R.T.: 18.633 min
Delta R.T.: -0.007 min
Response: 89217
Conc: 0.74 ug/ml

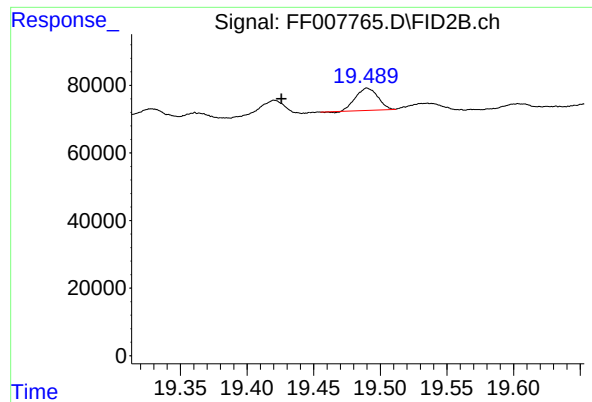

#15 N-TETRATRIACONTANE

R.T.: 19.490 min
Delta R.T.: 0.064 min
Response: 76444
Conc: 0.73 ug/ml

Instrument :
FID_G
ClientSampleId :