

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102720\
 Data File : FF007766.D
 Signal(s) : FID2B.ch
 Acq On : 27 Oct 2020 13:24
 Operator : DD\AJ
 Sample : L4512-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 28 00:57:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.727	1296453	10.302 ug/ml
Target Compounds			
4) N-TETRADECANE	8.231	488124	3.348 ug/ml
7) N-EICOSANE	12.696f	82293	0.554 ug/ml
10) N-TETRACOSANE	14.926	147043	1.019 ug/ml
14) N-DOTRIACONTANE	18.629	252682	2.100 ug/ml
15) N-TETRATRIACONTANE	19.487f	86265	0.821 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102720\
Data File : FF007766.D
Signal(s) : FID2B.ch
Acq On : 27 Oct 2020 13:24
Operator : DD\AJ
Sample : L4512-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 28 00:57:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

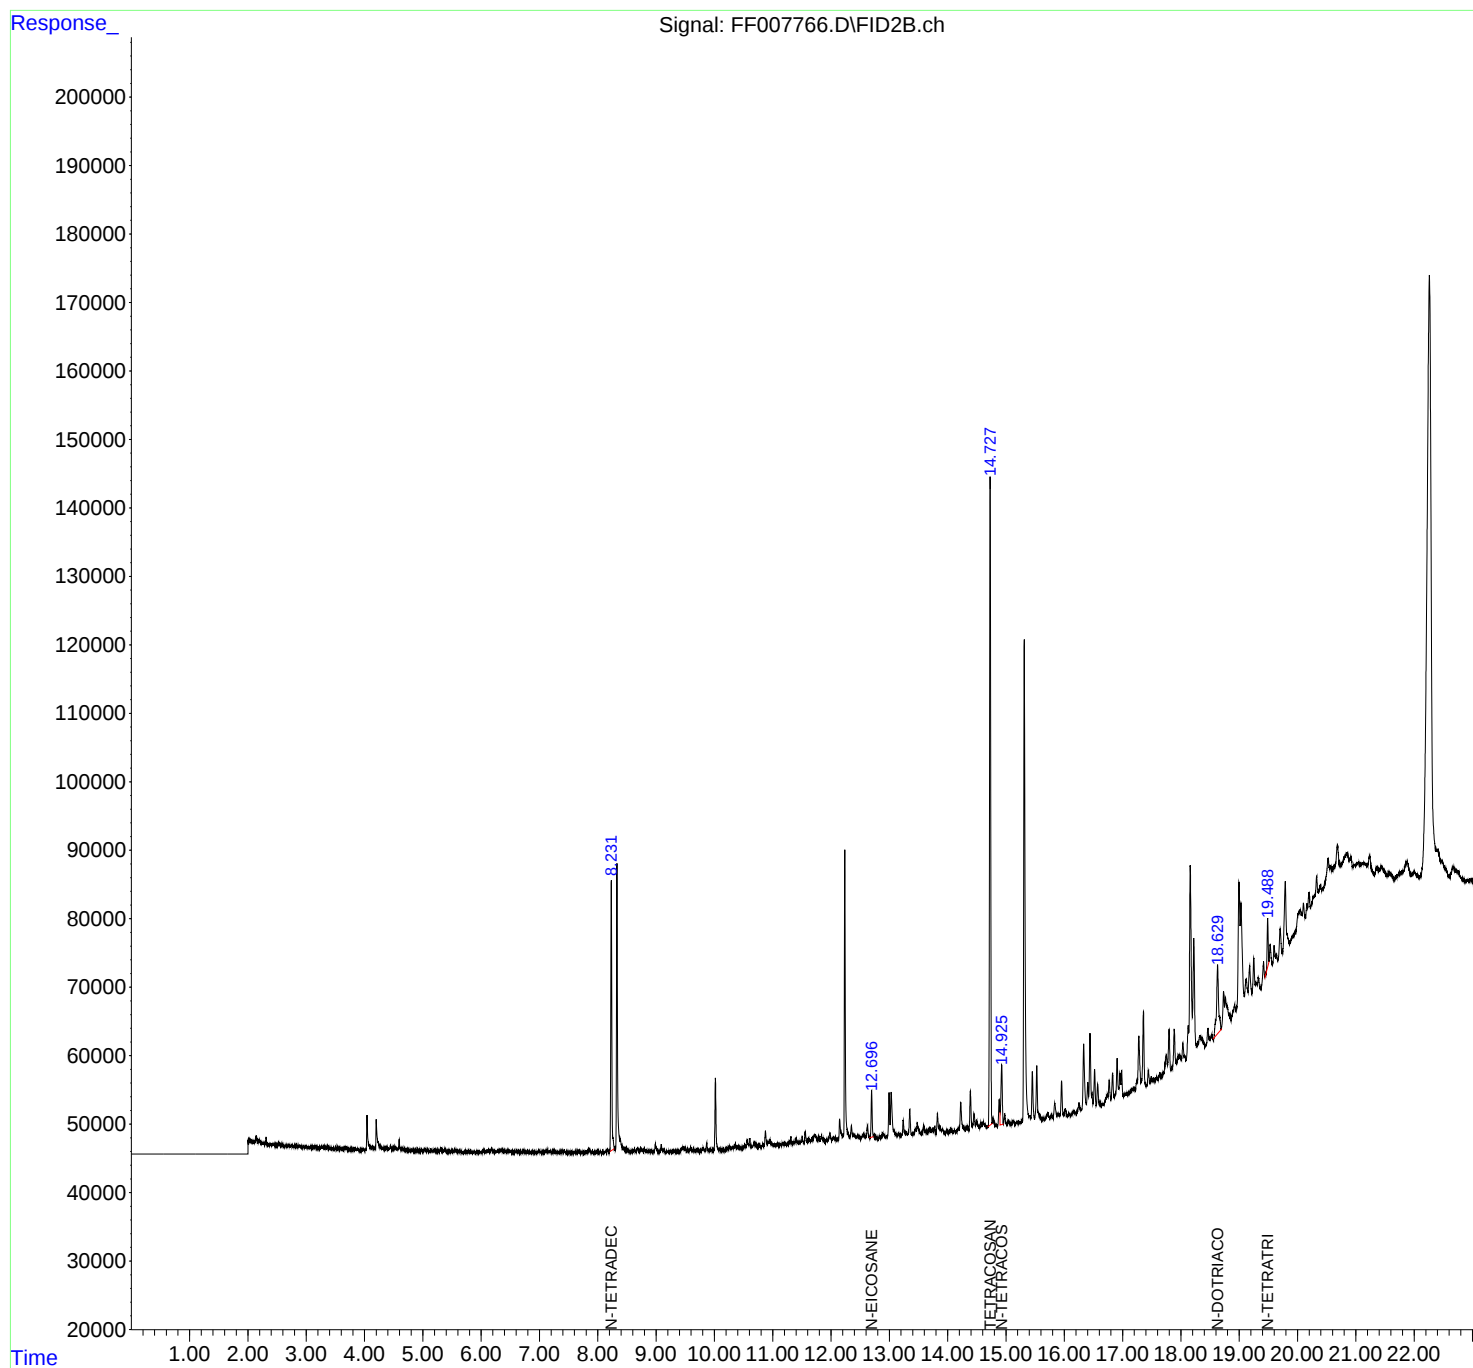


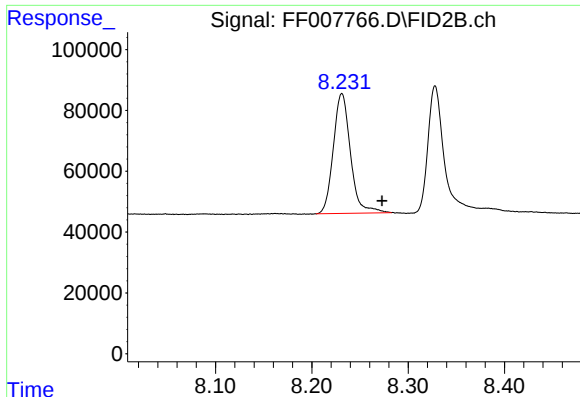

#4 N-TETRADECANE


R.T.: 8.231 min
Delta R.T.: -0.042 min
Response: 488124
Conc: 3.35 ug/ml

Instrument :
FID_G
ClientSampleId :

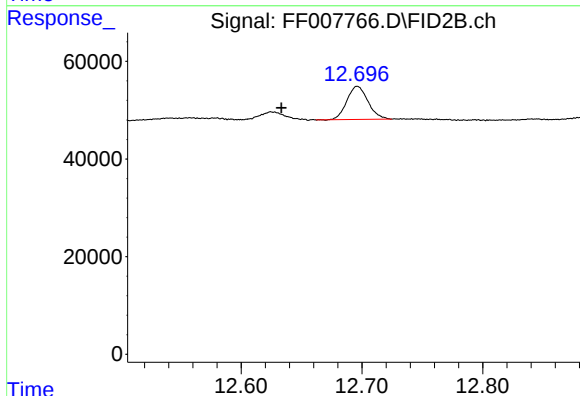


#7 N-EICOSANE

R.T.: 12.696 min
Delta R.T.: 0.063 min
Response: 82293
Conc: 0.55 ug/ml

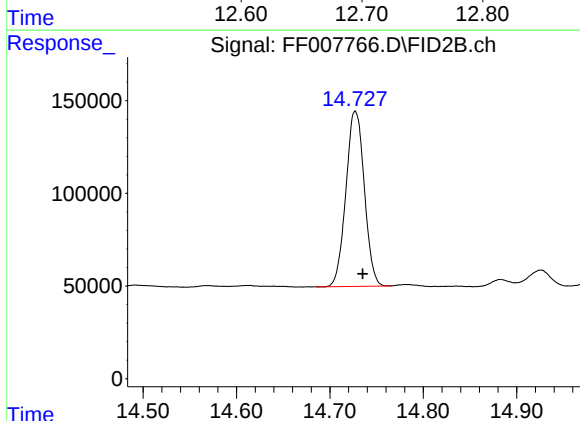


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.727 min
Delta R.T.: -0.008 min
Response: 1296453
Conc: 10.30 ug/ml

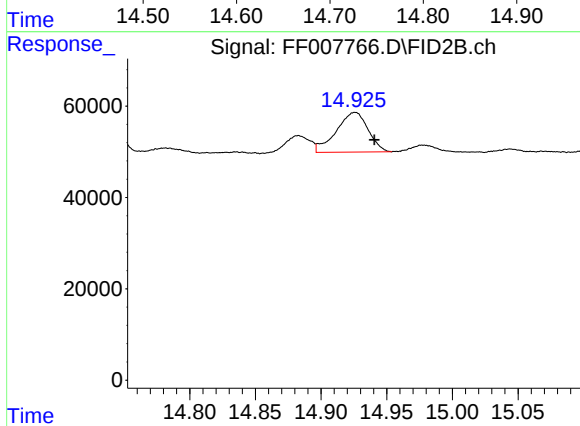

#10 N-TETRACOSANE


R.T.: 14.926 min
Delta R.T.: -0.015 min
Response: 147043
Conc: 1.02 ug/ml

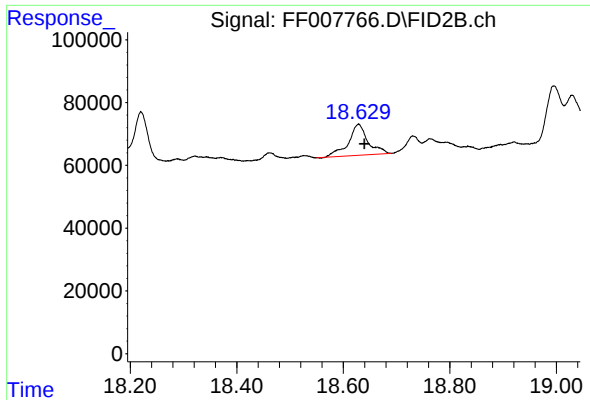

#14 N-DOTRIACONTANE

R.T.: 18.629 min
Delta R.T.: -0.011 min
Response: 252682
Conc: 2.10 ug/ml

Instrument :
FID_G
ClientSampleId :

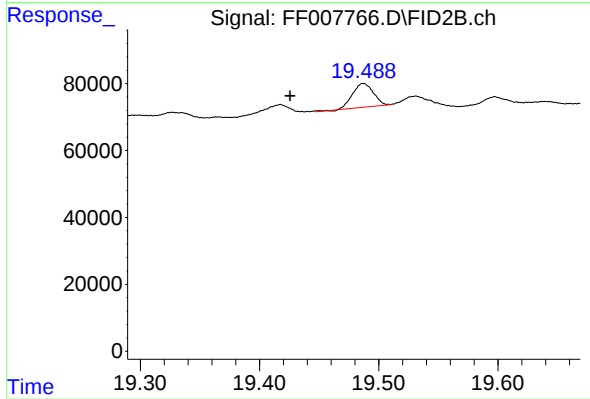

#15 N-TETRATRIACONTANE

R.T.: 19.487 min
Delta R.T.: 0.061 min
Response: 86265
Conc: 0.82 ug/ml